

Field Evaluation Kunak Air Lite



Background

- From 03/01/2024 to 05/01/2024, three **Kunak Air Lite** multi-sensor units were deployed at the South Coast AQMD stationary ambient monitoring site in Rubidoux and were run side-by-side with Federal Equivalent Method (FEM) and Federal Reference Method (FRM) instruments measuring the same pollutants.
- Kunak Air Lite (3 units tested):
 - Gas Sensors: **Electrochemical (Alphasense, non-FEM)**
 - PM – **Optical (Plantower PMS5003, non-FEM)**
 - Each unit measures: O₃ (ppb), NO₂ (ppb), PM_{1.0} (μg/m³), PM_{2.5} (μg/m³), PM₁₀ (μg/m³), T (°C), RH (%)
 - **Unit cost: \$5,033 as-tested (\$5,960 with cloud service)**
 - Time resolution: 1-min
 - Units IDs: 144, 145, and 146



- South Coast AQMD Reference instruments:
 - O₃ instrument (**Teledyne T400, hereinafter FEM T400**); **cost: ~\$7,000**
 - Time resolution; 1-min
 - NO/NO₂ instrument (**Teledyne T200, hereinafter FRM T200**); **cost: ~\$11,000**
 - Time resolution: 1-min
 - PM instrument (**Teledyne API T640; FEM PM_{2.5}, hereinafter FEM T640**); **cost: \$21,000**
 - Time resolution: 1-min
 - Measures PM_{1.0}, PM_{2.5}, PM₁₀ (μg/m³)
 - PM Instrument (**MetOne BAM; FEM PM_{2.5} and PM₁₀, hereinafter FEM BAM**); **cost: \$25,000 and up**
 - Time resolution: 1-hr
 - Measures PM_{2.5}, PM₁₀ (μg/m³)
 - Met station (T, RH, P, WS, WD); **cost: ~\$5,000**
 - Time resolution: 1-min


**Ozone (O_3)
in Kunak Air Lite**

Data validation & recovery


- Basic QA/QC procedures were used to validate the collected data (i.e., obvious outliers, negative values, and invalid data-points were eliminated from the data-set)
- Data recovery for O₃ from Unit 144, Unit 145 and Unit 146 was ~98.9%, ~99.1% and ~99.1%, respectively
- Values below manufacturer stated limit of detection were excluded from further analysis but do not count against data recovery

Kunak Air Lite; Intra-model variability




- Absolute intra-model variability was ~1.09 ppb for the ozone measurements (calculated as the standard deviation of the three sensor means)
- Relative intra-model variability was ~2.86% for the ozone measurements (calculated as the absolute intra-model variability relative to the mean of the three sensor means)

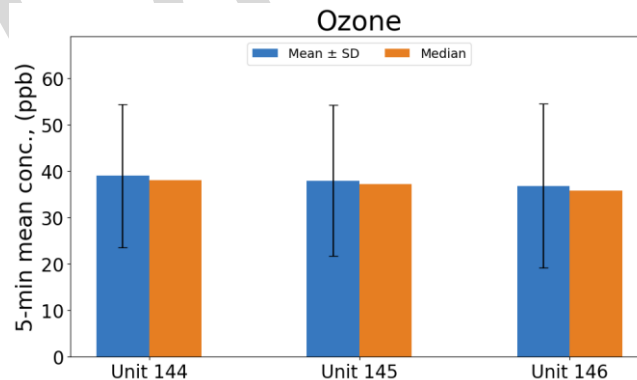


Kunak Air Lite vs FEM T400 (Ozone; 5-min mean)

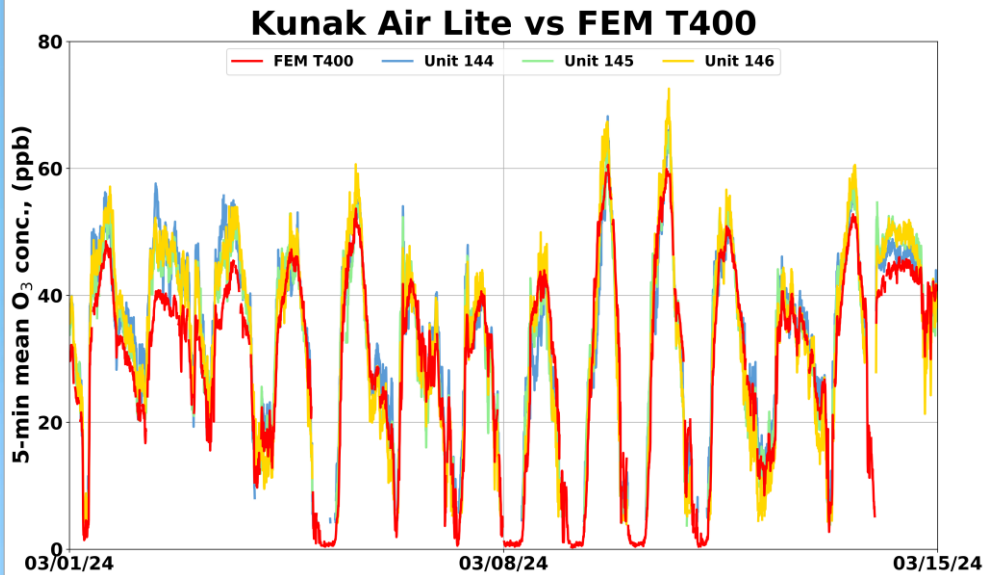




- The Kunak Air Lite sensors showed strong correlation with the corresponding FEM T400 ozone data ($0.84 < R^2 < 0.89$)
- Overall, the Kunak Air Lite sensors underestimated the ozone concentration as measured by the FEM T400 ozone instrument
- The Kunak Air Lite sensors seemed to track the diurnal ozone variations as recorded by the FEM T400 instrument

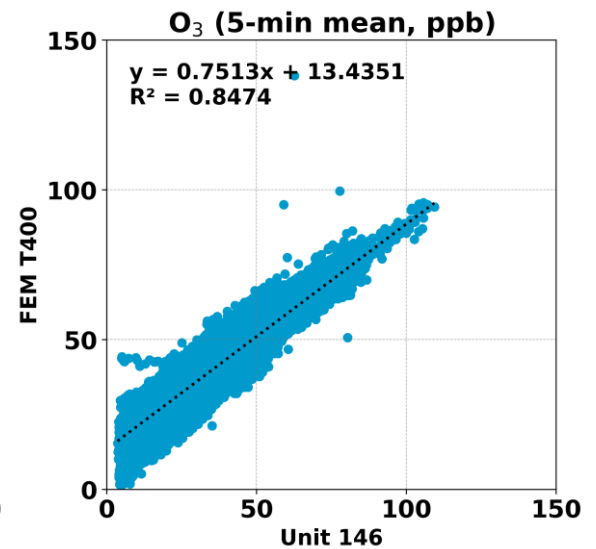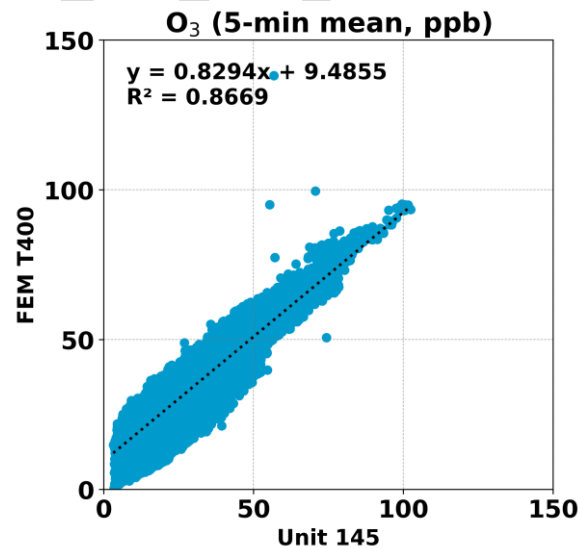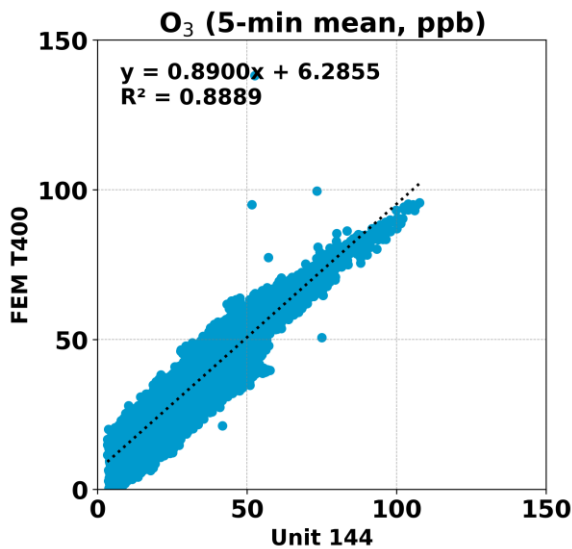


Kunak Air Lite vs FEM T400 (Ozone; 1-hr mean)

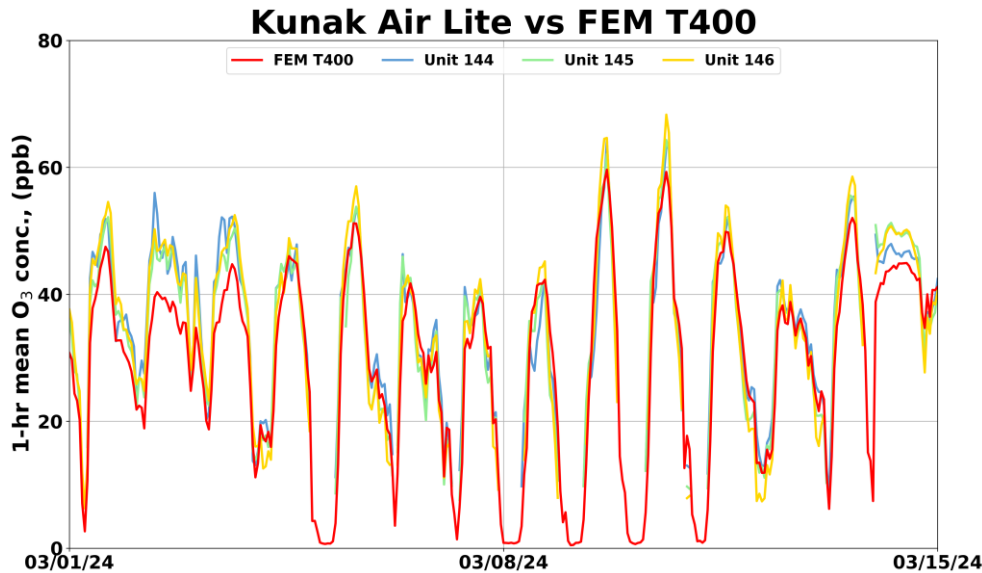




- The Kunak Air Lite sensors showed strong correlation with the corresponding FEM T400 ozone data ($0.85 < R^2 < 0.90$)
- Overall, the Kunak Air Lite sensors underestimated the ozone concentration as measured by the FEM T400 ozone instrument
- The Kunak Air Lite sensors seemed to track the diurnal ozone variations as recorded by the FEM T400 instrument

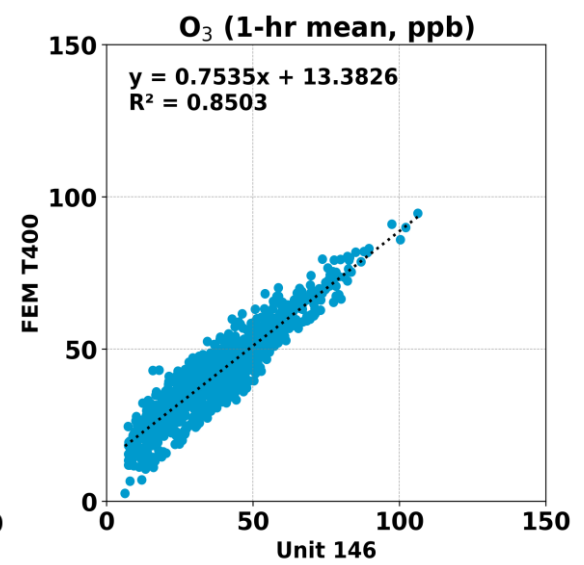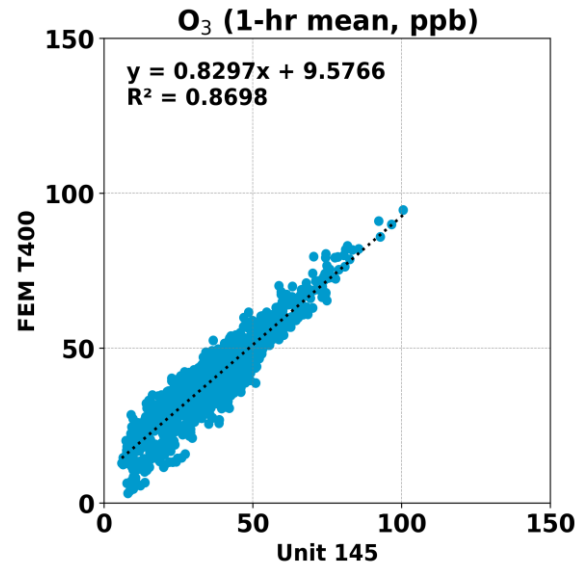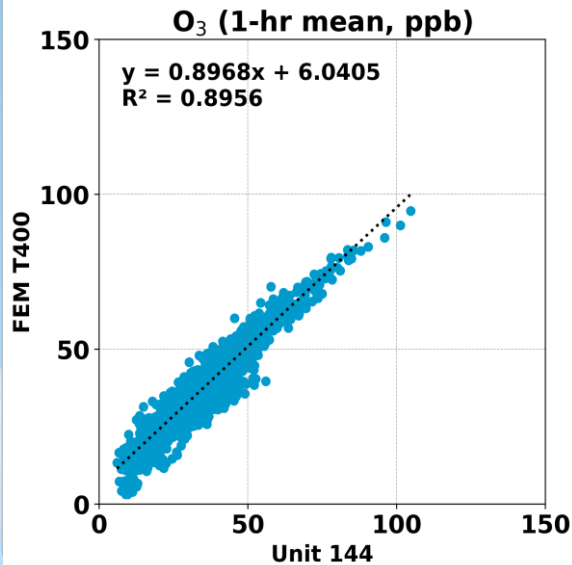

Kunak Air Lite vs FEM T400 (Ozone; 8-hr mean)

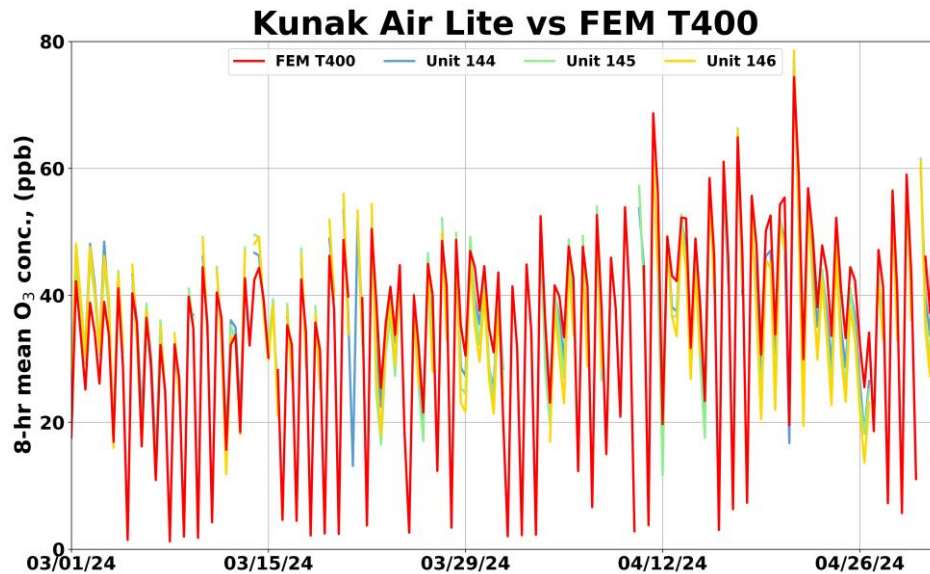

- The Kunak Air Lite sensors showed strong correlation with the corresponding FEM T400 ozone data ($0.78 < R^2 < 0.88$)
- Overall, the Kunak Air Lite sensors underestimated the ozone concentration as measured by the FEM T400 ozone instrument
- The Kunak Air Lite sensors seemed to track the diurnal ozone variations as recorded by the FEM T400 instrument

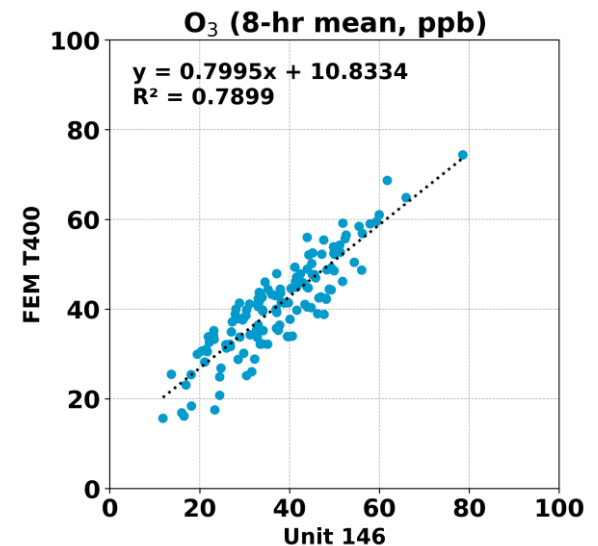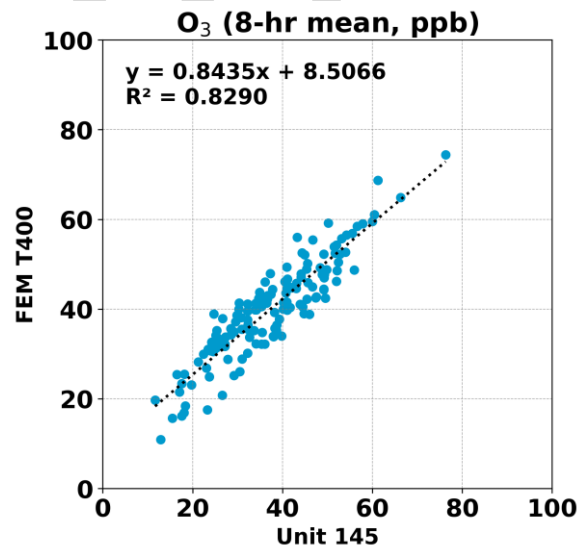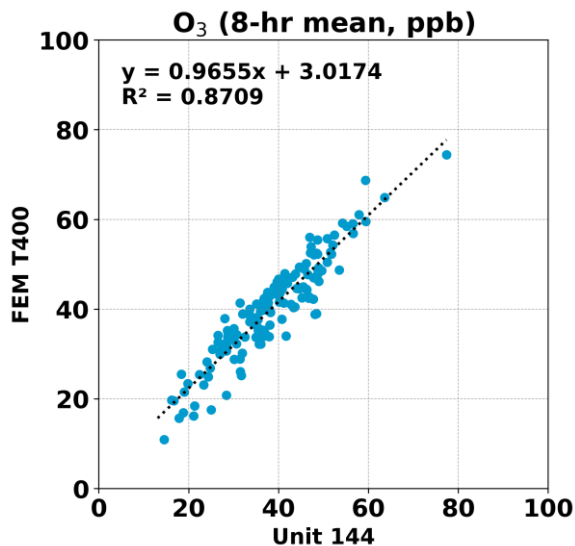

Summary: Ozone

	Average of 3 Sensors, Ozone		Kunak Air Lite vs FEM T400, Ozone						FEM T400, Ozone (ppb)		
	Average (ppb)	SD (ppb)	R ²	Slope	Intercept	MBE ¹ (ppb)	MAE ² (ppb)	RMSE ³ (ppb)	FEM T400 Average	FEM T400 SD	Range during the field evaluation
5-min	37.0	17.1	0.85 to 0.89	0.75 to 0.89	6.3 to 13.4	-4.1 to -2.1	4.7 to 6.8	5.9 to 8.2	35.1	19.2	0.1 to 138.1
1-hr	37.5	16.5	0.85 to 0.90	0.75 to 0.90	6.1 to 13.4	-4.2 to -2.1	4.5 to 6.7	5.5 to 8.0	34.0	19.2	0.5 to 94.6
8-hr	38.0	11.7	0.79 to 0.87	0.80 to 0.97	3.0 to 10.8	-3.4 to -1.7	3.7 to 5.4	4.3 to 6.3	34.1	16.3	1.2 to 74.4

¹ Mean Bias Error (MBE): the difference between the sensors and the reference instruments. MBE indicates the tendency of the sensors to underestimate (negative MBE values) or overestimate (positive MBE values).

² Mean Absolute Error (MAE): the absolute difference between the sensors and the reference instruments. The larger MAE values, the higher measurement errors as compared to the reference instruments.

³ Root Mean Square Error (RMSE): another metric to calculate measurement errors.


**Nitrogen Dioxide (NO₂)
in Kunak Air Lite**

Data validation & recovery


- Basic QA/QC procedures were used to validate the collected data (i.e., obvious outliers, negative values, and invalid data-points were eliminated from the data-set)
- Data recovery for NO₂ from Unit 144, Unit 145 and Unit 146 was ~99.0%, ~99.1% and ~99.2%, respectively
- Values below manufacturer stated limit of detection were excluded from further analysis but do not count against data recovery

Kunak Air Lite; Intra-model variability




- Absolute intra-model variability was ~0.41 ppb for the NO₂ measurements (calculated as the standard deviation of the three sensor means)
- Relative intra-model variability was ~3.21% for the NO₂ measurements (calculated as the absolute intra-model variability relative to the mean of the three sensor means)

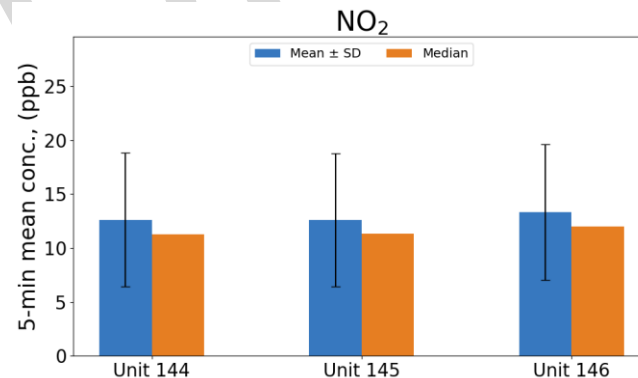


Kunak Air Lite vs FRM T200 (NO₂; 5-min mean)

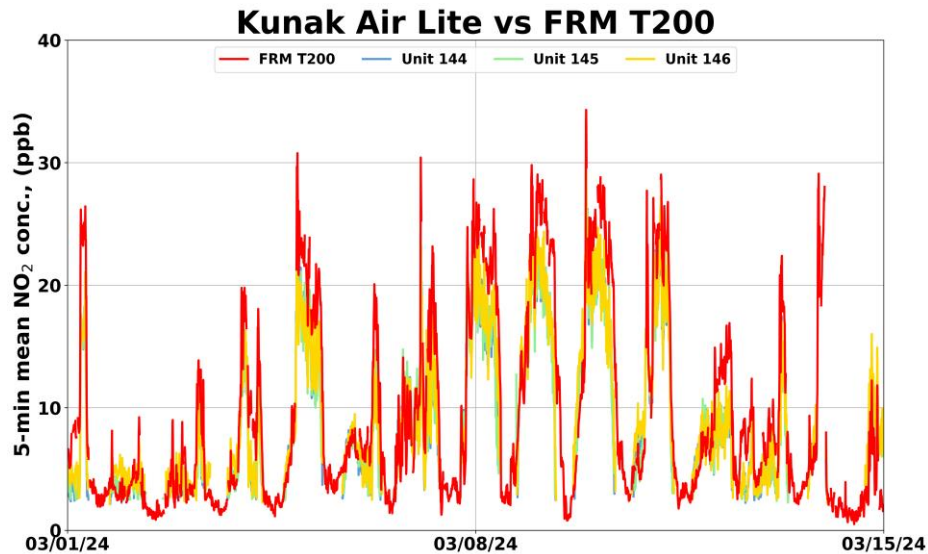




- The Kunak Air Lite sensors showed moderate correlations with the corresponding FRM T200 NO₂ data ($0.66 < R^2 < 0.70$)
- Overall, the Kunak Air Lite sensors overestimated the NO₂ concentration as measured by the FRM T200 instrument
- The Kunak Air Lite sensors seemed to track the diurnal NO₂ variations as recorded by the FRM T200 instrument

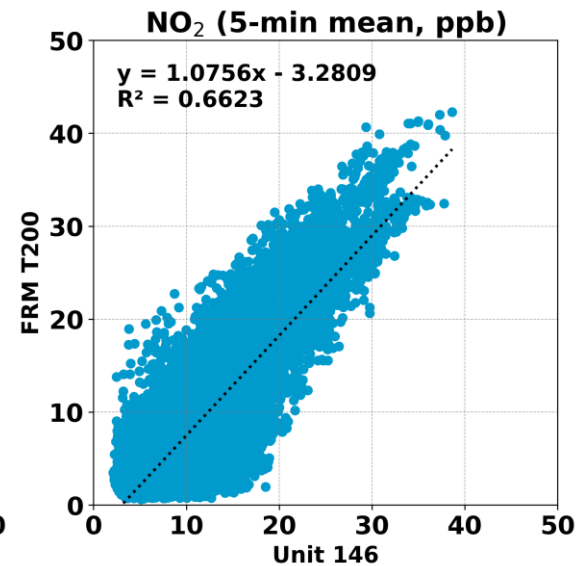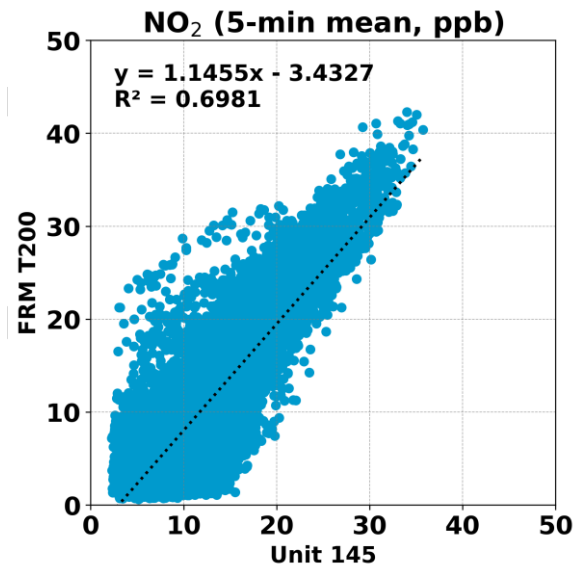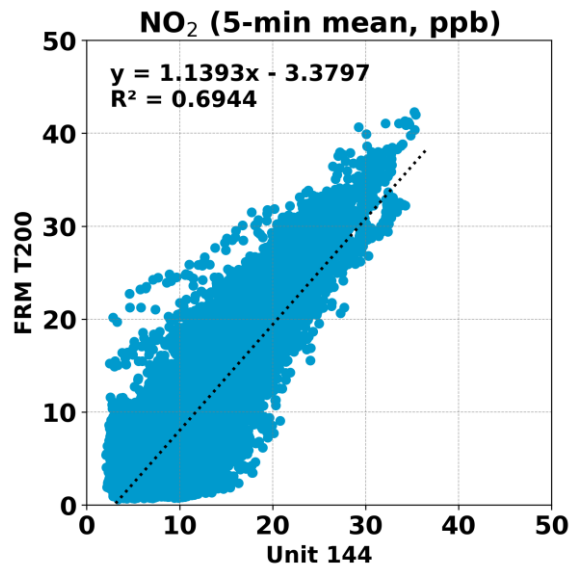


Kunak Air Lite vs FRM T200 (NO₂; 1-hr mean)

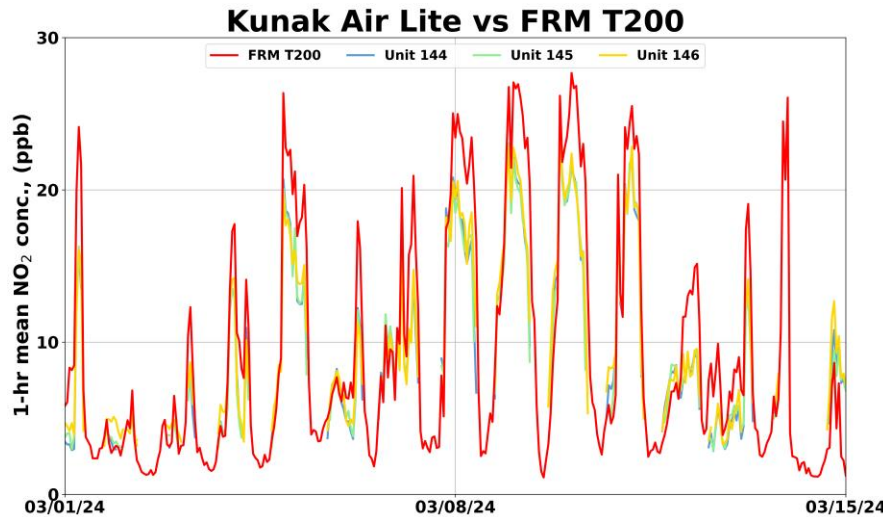




- The Kunak Air Lite sensors showed moderate to strong correlations with the corresponding FRM T200 NO₂ data ($0.68 < R^2 < 0.73$)
- Overall, the Kunak Air Lite sensors overestimated the NO₂ concentration as measured by the FRM T200 instrument
- The Kunak Air Lite sensors seemed to track the diurnal NO₂ variations as recorded by the FRM T200 instrument

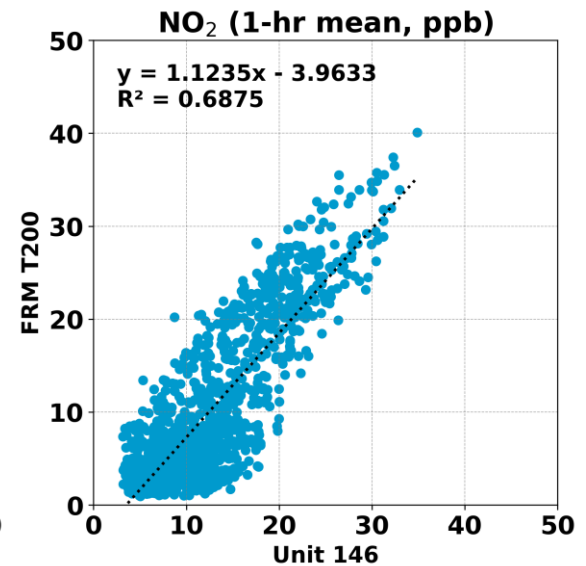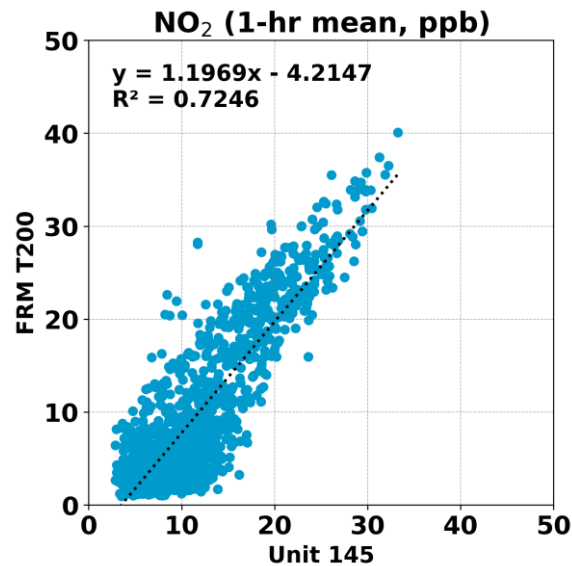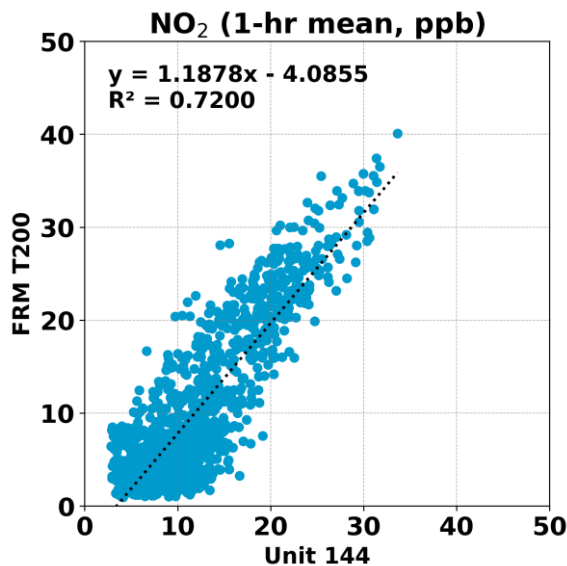

Kunak Air Lite vs FRM T200 (NO₂; 24-hr mean)

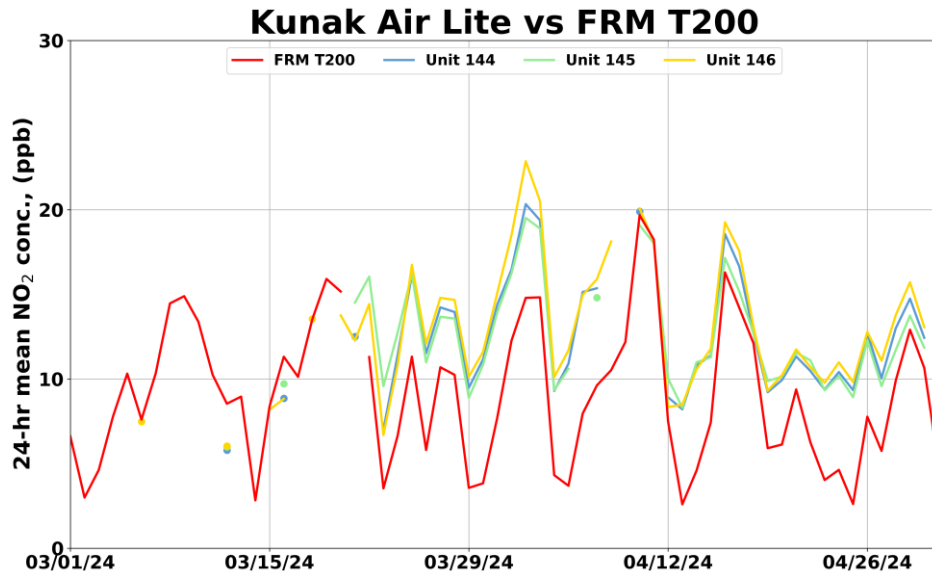

- The Kunak Air Lite sensors showed moderate to strong correlations with the corresponding FRM T200 NO₂ data ($0.57 < R^2 < 0.71$)
- Overall, the Kunak Air Lite sensors overestimated the NO₂ concentration as measured by the FRM T200 instrument
- The Kunak Air Lite sensors seemed to track the daily NO₂ variations as recorded by the FRM T200 instrument

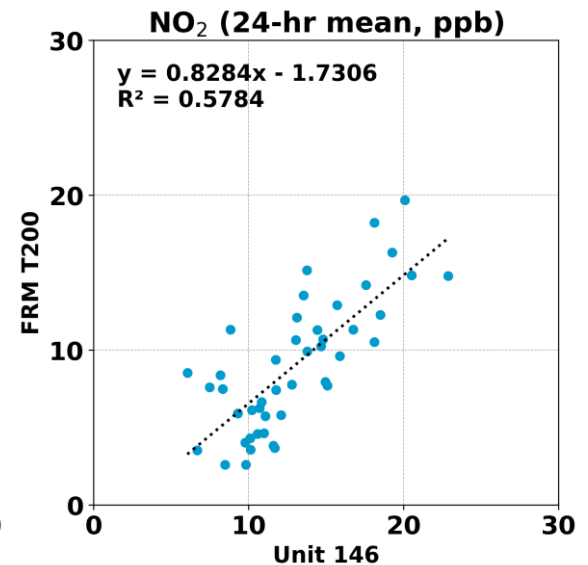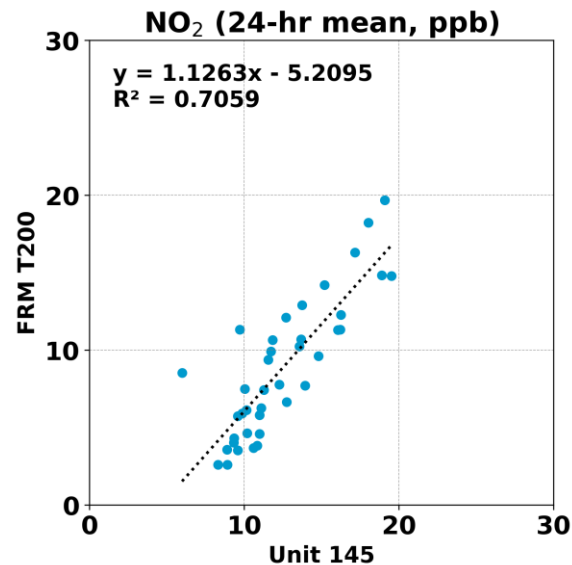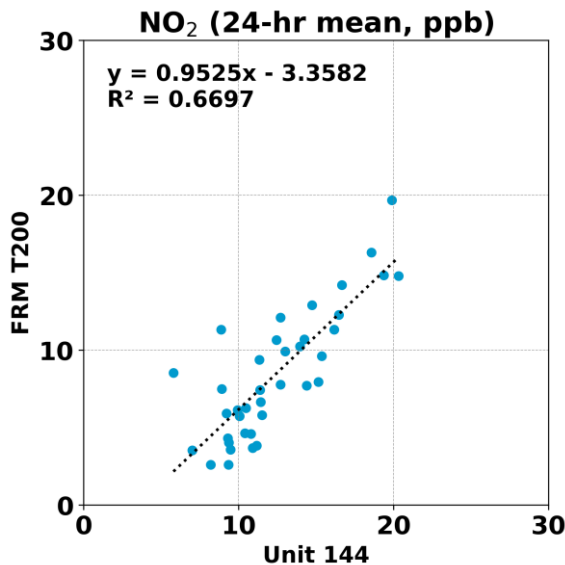

Summary: NO₂

	Average of 3 Sensors, NO ₂		Kunak Air Lite vs FRM T200, NO ₂						FRM T200, NO ₂ (ppb)		
	Average (ppb)	SD (ppb)	R ²	Slope	Intercept	MBE ¹ (ppb)	MAE ² (ppb)	RMSE ³ (ppb)	FRM T200 Average	FRM T200 SD	Range during the field evaluation
5-min	12.5	6.3	0.66 to 0.70	1.08 to 1.15	-3.4 to -3.3	1.7 to 2.3	4.2 to 4.5	5.0 to 5.4	9.1	8.1	0.5 to 42.3
1-hr	12.6	6.1	0.69 to 0.72	1.12 to 1.20	-4.2 to -4.0	1.7 to 2.4	4.1 to 4.4	4.9 to 5.3	9.4	8.1	1.0 to 40.1
24-hr	12.6	3.6	0.58 to 0.71	0.83 to 1.13	-5.2 to -1.7	3.6 to 4.0	3.9 to 4.3	4.4 to 4.9	9.1	4.2	2.6 to 19.7

¹ Mean Bias Error (MBE): the difference between the sensors and the reference instruments. MBE indicates the tendency of the sensors to underestimate (negative MBE values) or overestimate (positive MBE values).

² Mean Absolute Error (MAE): the absolute difference between the sensors and the reference instruments. The larger MAE values, the higher measurement errors as compared to the reference instruments.

³ Root Mean Square Error (RMSE): another metric to calculate measurement errors.


**Particulate Matter (PM)
in Kunak Air Lite**

Data validation & recovery

- Basic QA/QC procedures were used to validate the collected data (i.e. obvious outliers, negative values and invalid data-points were eliminated from the data-set)
- Data recovery from Unit 144, Unit 145 and Unit 146 was ~99.5%, ~99.8% and ~99.9%, respectively for all PM measurements
- Values below manufacturer stated limit of detection were excluded from further analysis but do not count against data recovery



Kunak Air Lite; intra-model variability

- Absolute intra-model variability was ~0.57, ~0.68 and ~0.72 $\mu\text{g}/\text{m}^3$ for $\text{PM}_{1.0}$, $\text{PM}_{2.5}$ and PM_{10} , respectively (calculated as the standard deviation of the three sensor means)
- Relative intra-model variability was ~12.09%, ~8.75% and ~8.37% for $\text{PM}_{1.0}$, $\text{PM}_{2.5}$ and PM_{10} , respectively (calculated as the absolute intra-model variability relative to the mean of the three sensor means)

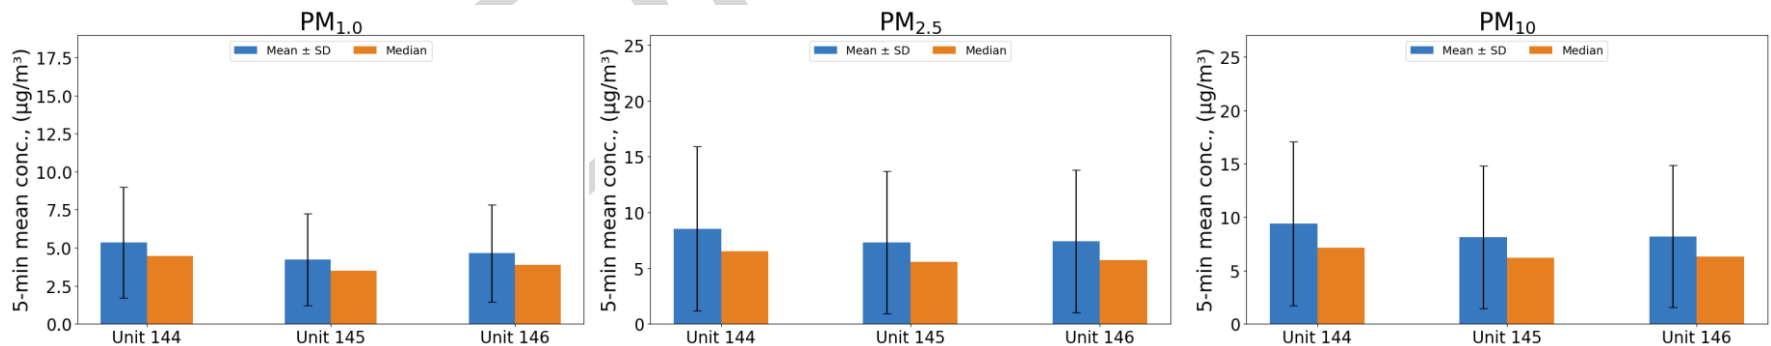



Reference Instruments: PM_{2.5} FEM BAM and FEM T640

- Data recovery for PM_{2.5} from FEM BAM and FEM T640 was ~ 99.1% and 99.9%, respectively.
- Strong correlations between the reference instruments for PM_{2.5} measurements ($R^2 \sim 0.77$) were observed.

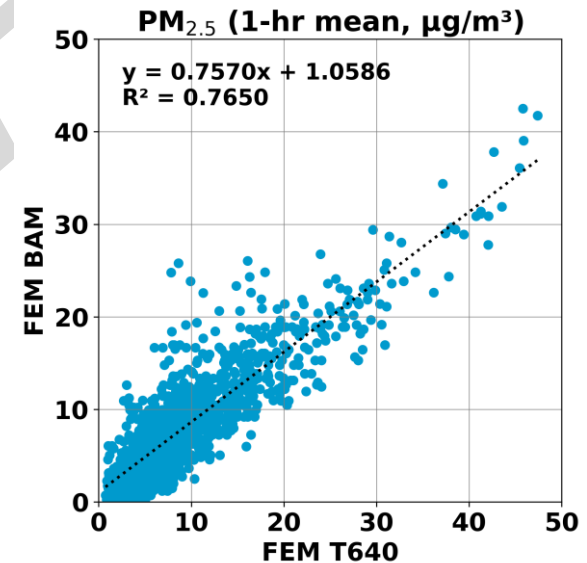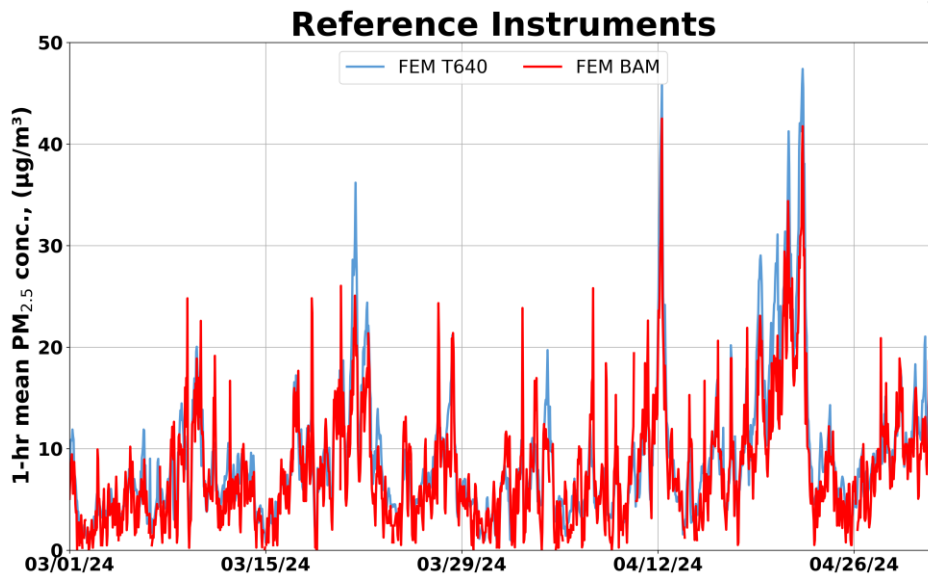


Reference Instruments: PM₁₀ FEM BAM and T640




- Data recovery for PM₁₀ from FEM BAM and T640 was ~ 98.9% and 99.9%, respectively.
- Strong correlations between the reference instruments for PM₁₀ measurements ($R^2 \sim 0.83$) were observed.

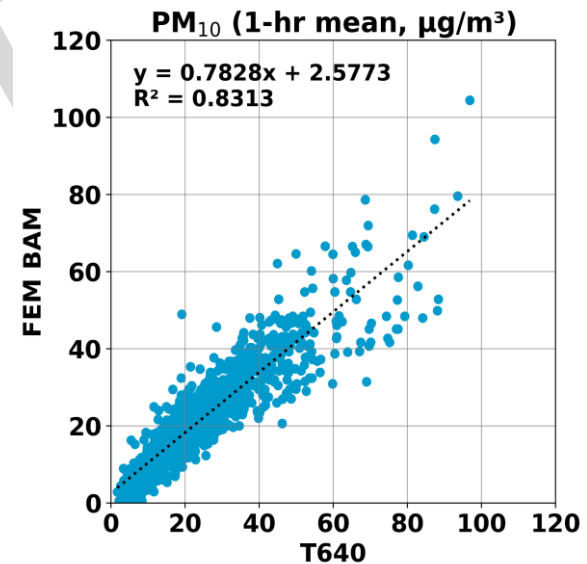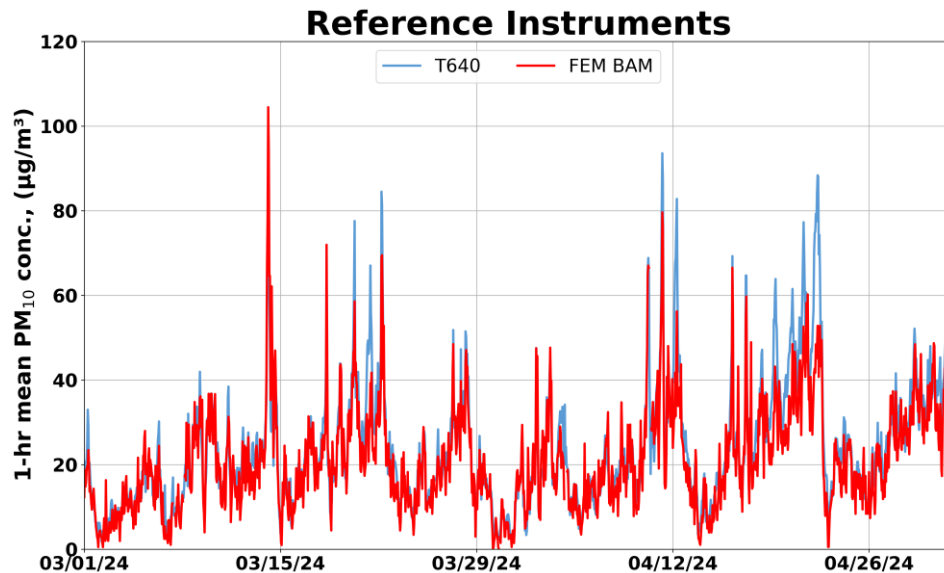

Kunak Air Lite vs T640 (PM_{1.0}; 5-min mean)

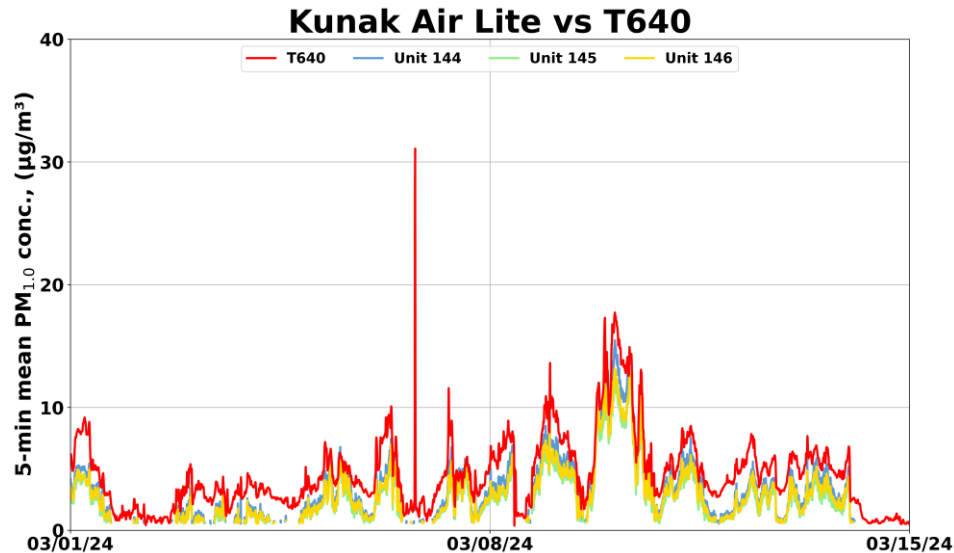


- The Kunak Air Lite sensors showed strong correlations with the corresponding T640 data ($0.76 < R^2 < 0.79$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{1.0} mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM_{1.0} diurnal variations as recorded by T640

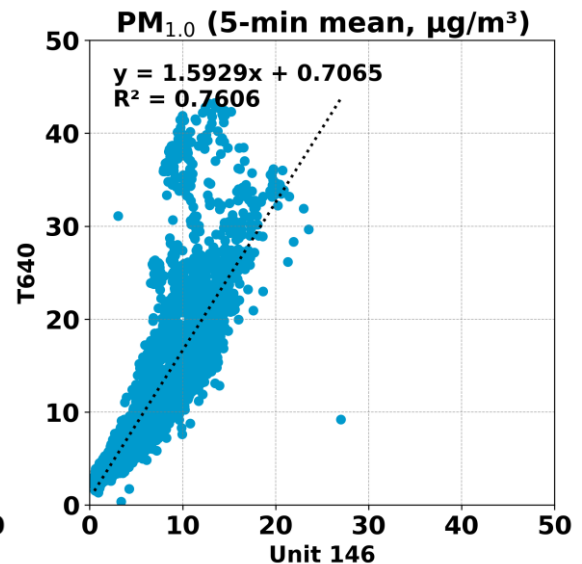
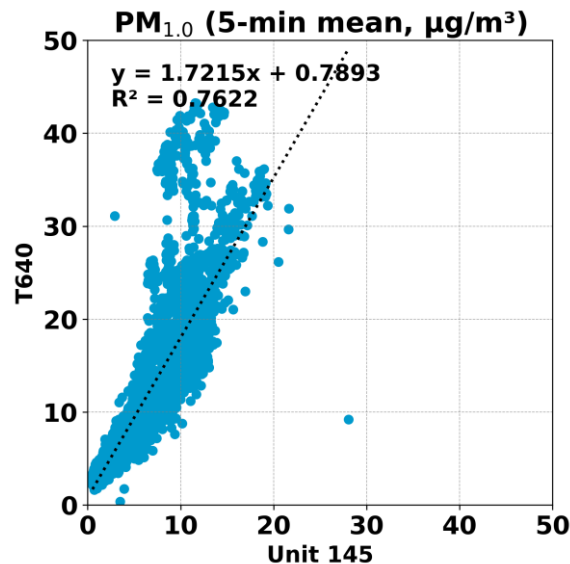
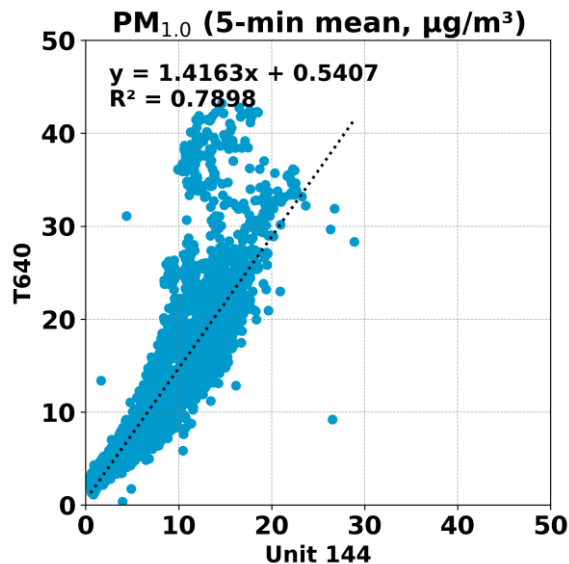


Kunak Air Lite vs FEM T640 (PM_{2.5}; 5-min mean)


Kunak Air Lite vs FEM T640

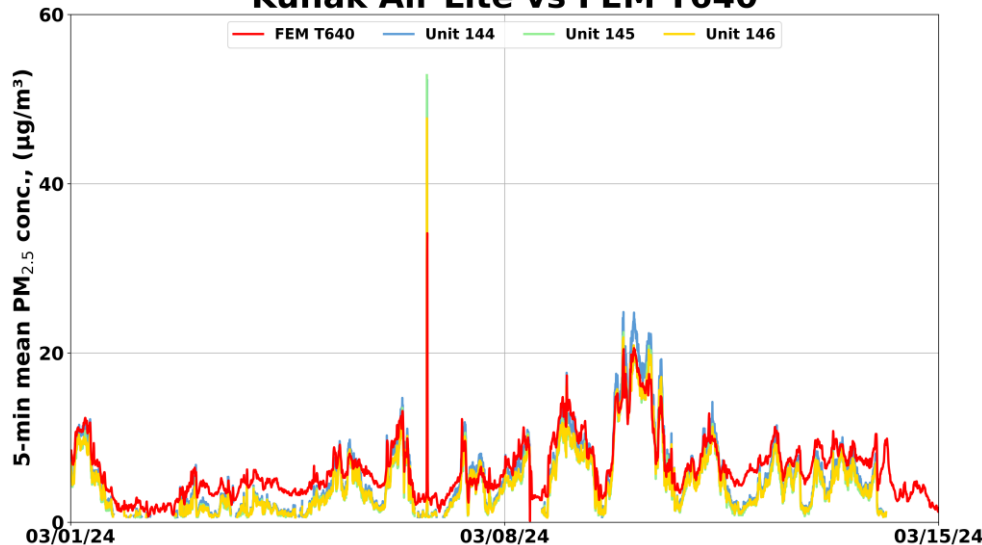




- The Kunak Air Lite sensors showed strong to very strong correlations with the corresponding FEM T640 data ($0.88 < R^2 < 0.91$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{2.5} mass concentrations as measured by FEM T640
- The Kunak Air Lite sensors seemed to track the PM_{2.5} diurnal variations as recorded by FEM T640

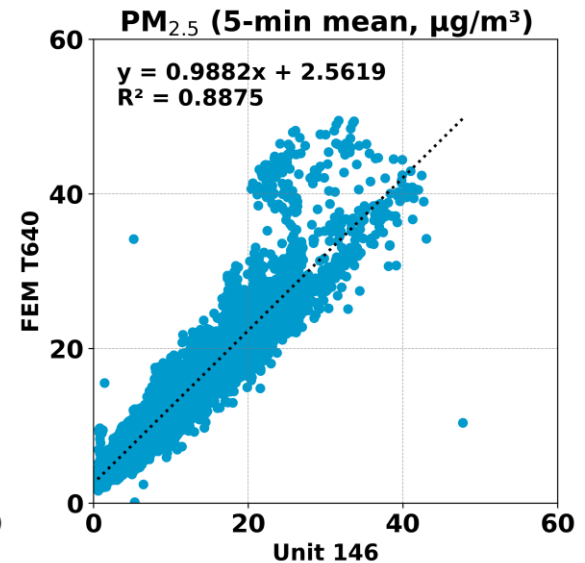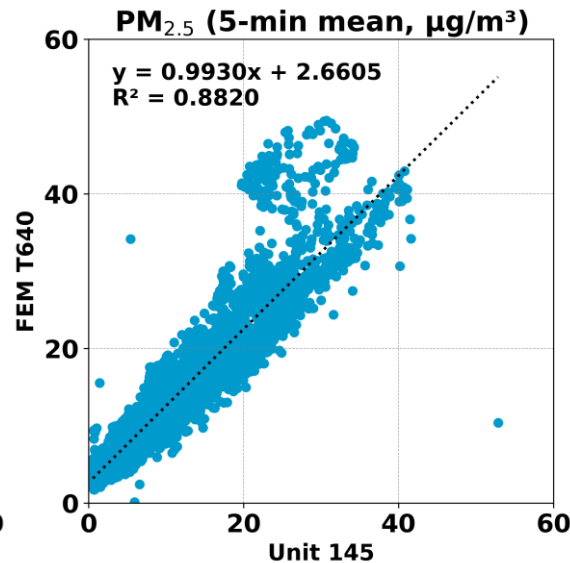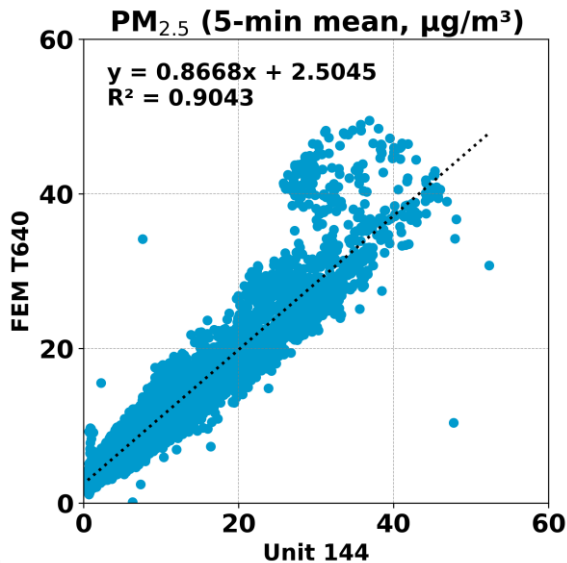


Kunak Air Lite vs T640 (PM₁₀; 5-min mean)

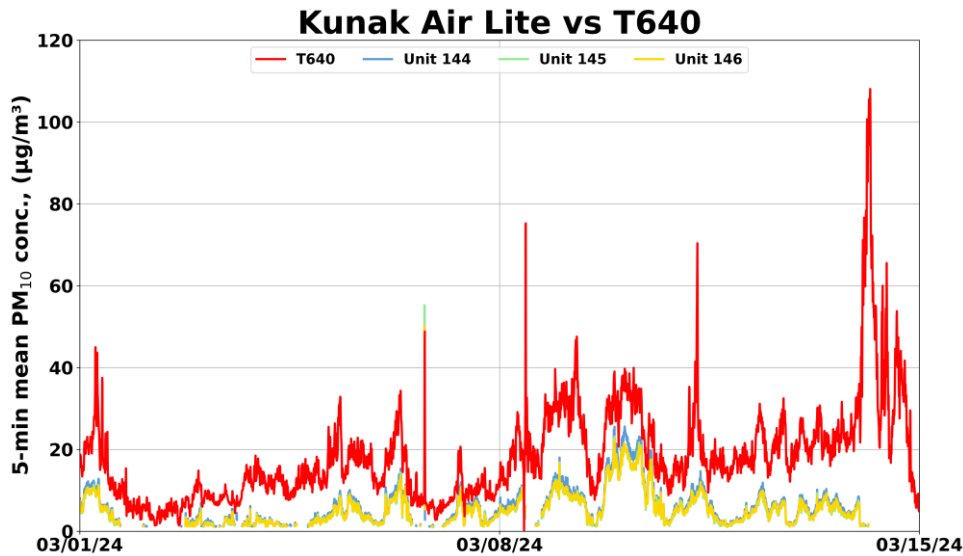




- The Kunak Air Lite sensors showed moderate correlations with the corresponding T640 data ($0.60 < R^2 < 0.63$)
- Overall, the Kunak Air Lite sensors underestimated the PM₁₀ mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM₁₀ diurnal variations as recorded by T640

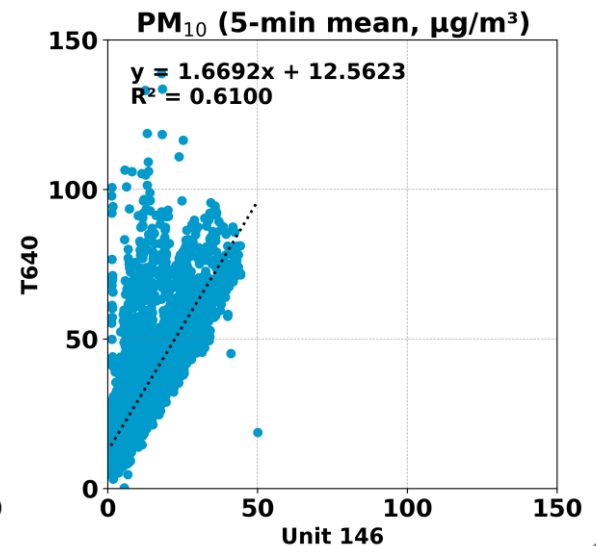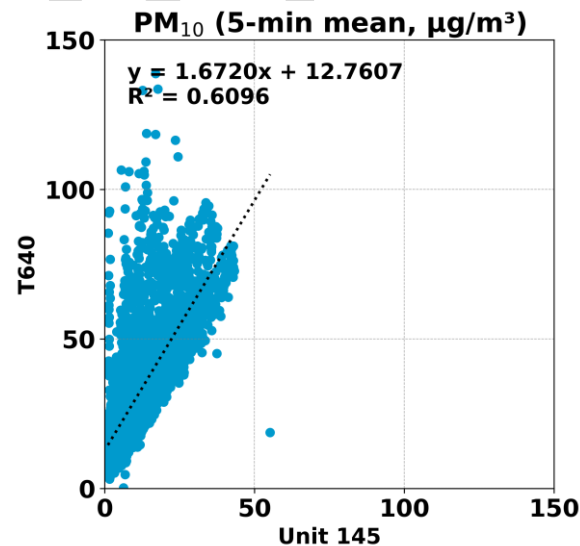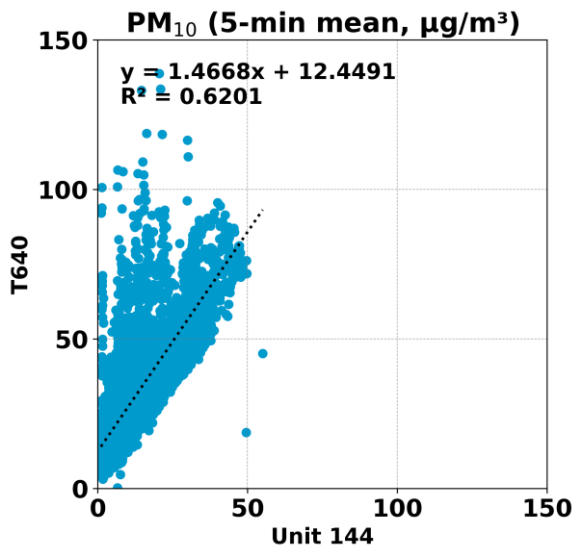


Kunak Air Lite vs T640 (PM_{1.0}; 1-hr mean)

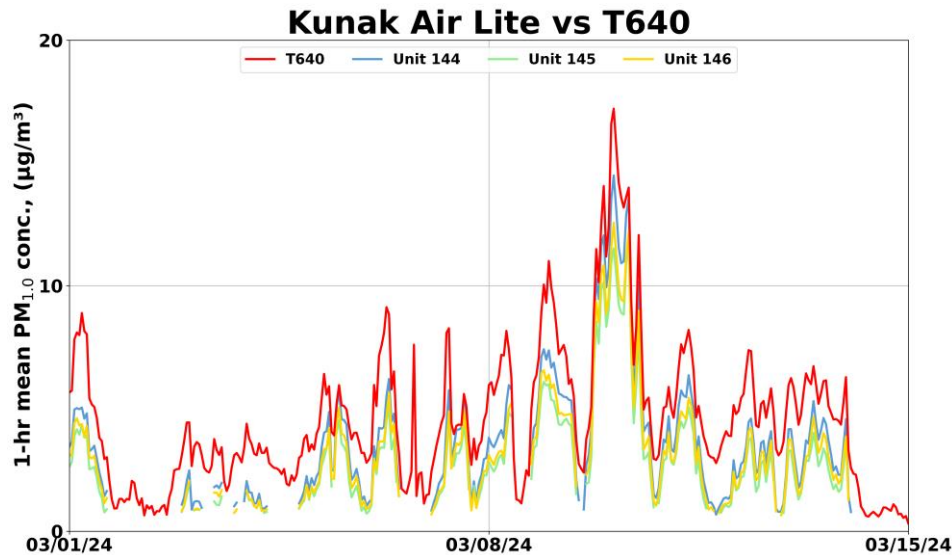




- The Kunak Air Lite sensors showed strong correlations with the corresponding T640 data ($0.77 < R^2 < 0.80$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{1.0} mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM_{1.0} diurnal variations as recorded by T640

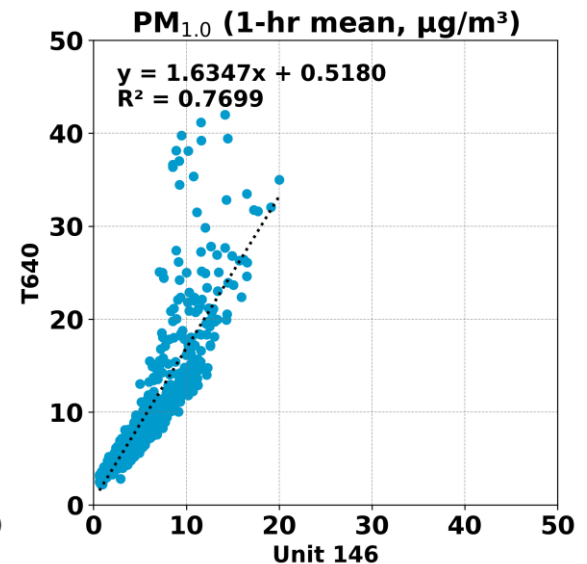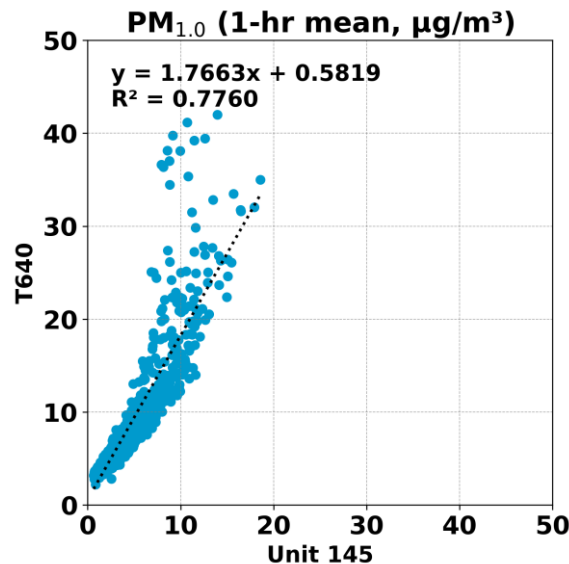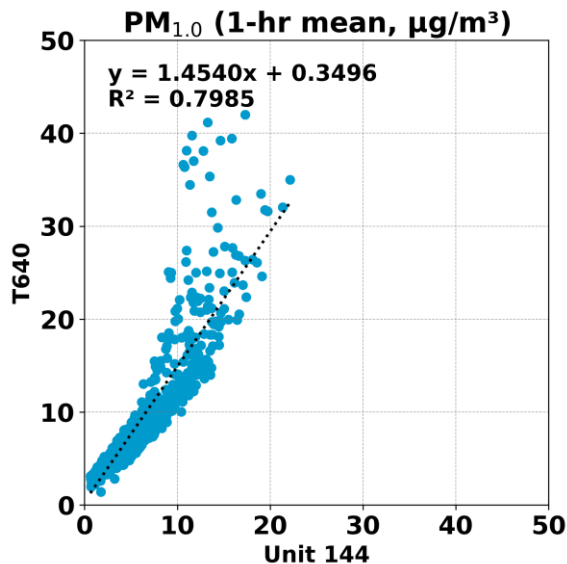


Kunak Air Lite vs FEM T640 (PM_{2.5}; 1-hr mean)

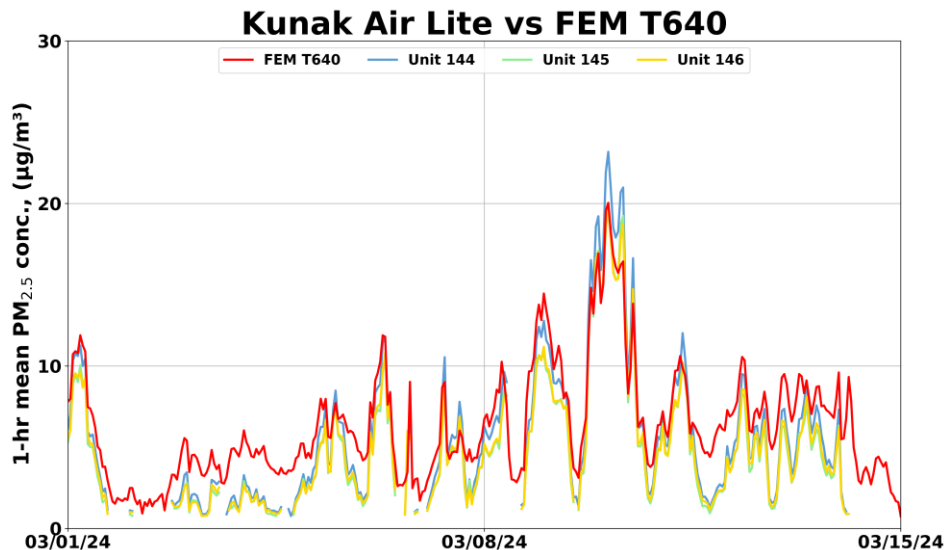




- The Kunak Air Lite sensors showed strong to very strong correlations with the corresponding FEM T640 data ($0.89 < R^2 < 0.92$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{2.5} mass concentrations as measured by FEM T640
- The Kunak Air Lite sensors seemed to track the PM_{2.5} diurnal variations as recorded by FEM T640

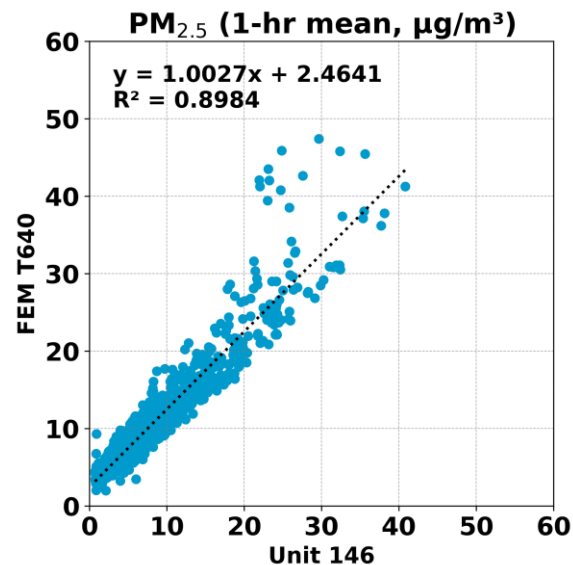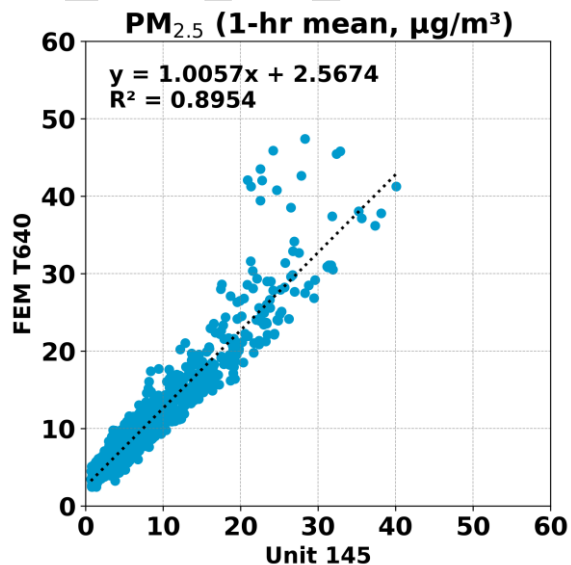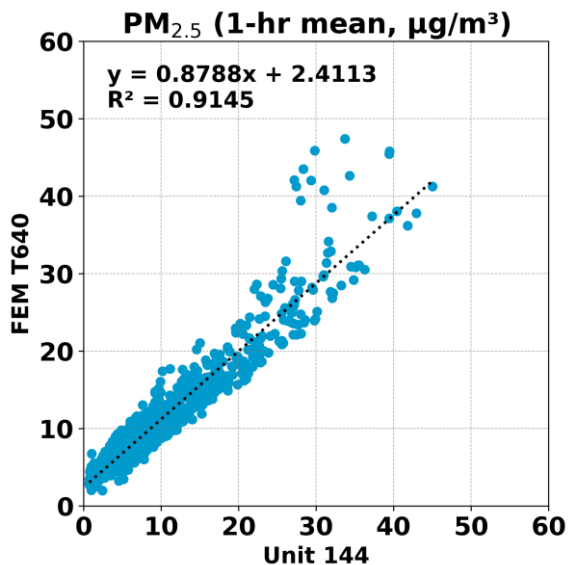


Kunak Air Lite vs T640 (PM₁₀; 1-hr mean)

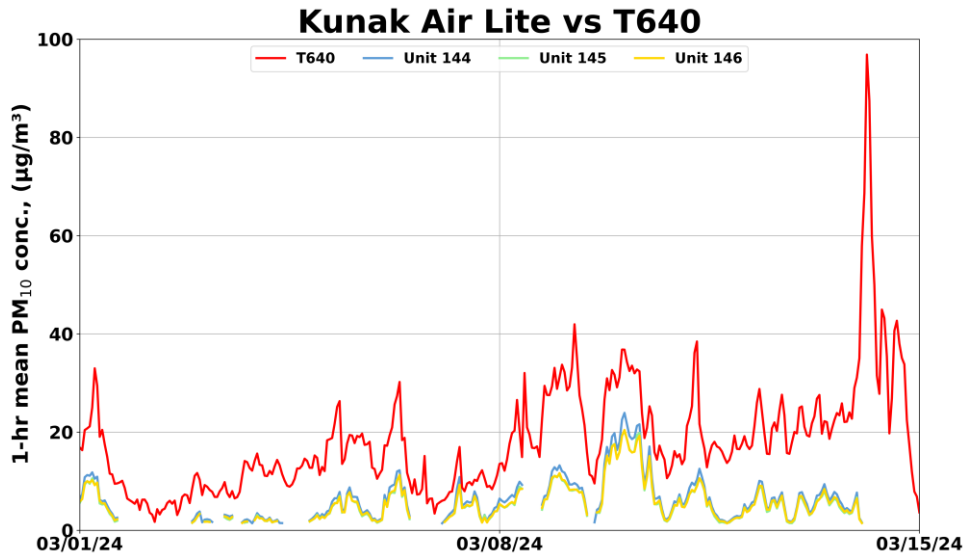




- The Kunak Air Lite sensors showed moderate correlations with the corresponding T640 data ($0.64 < R^2 < 0.67$)
- Overall, the Kunak Air Lite sensors underestimated the PM₁₀ mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM₁₀ diurnal variations as recorded by T640

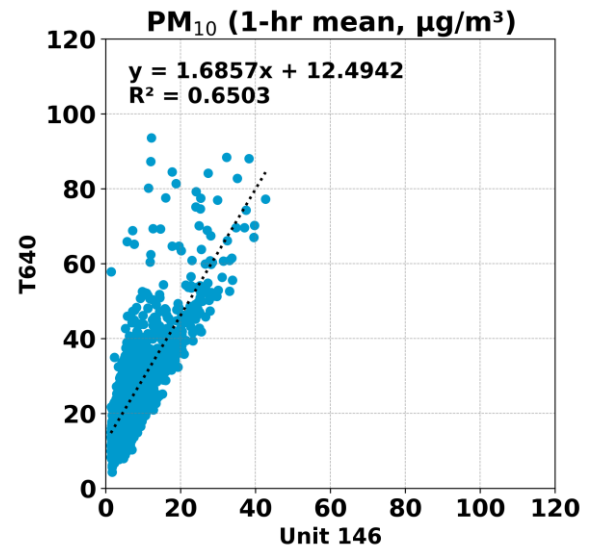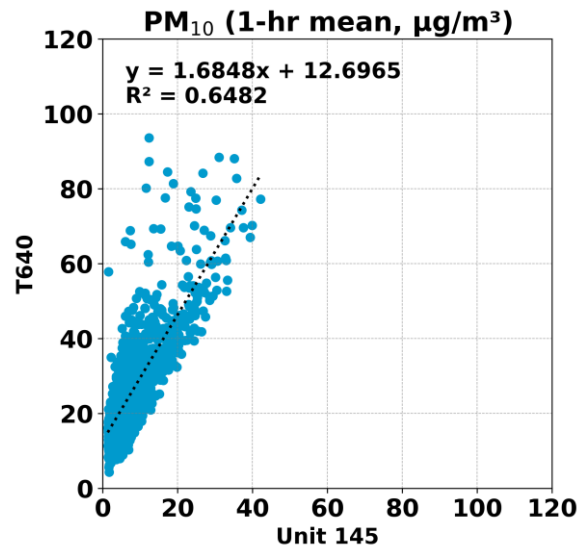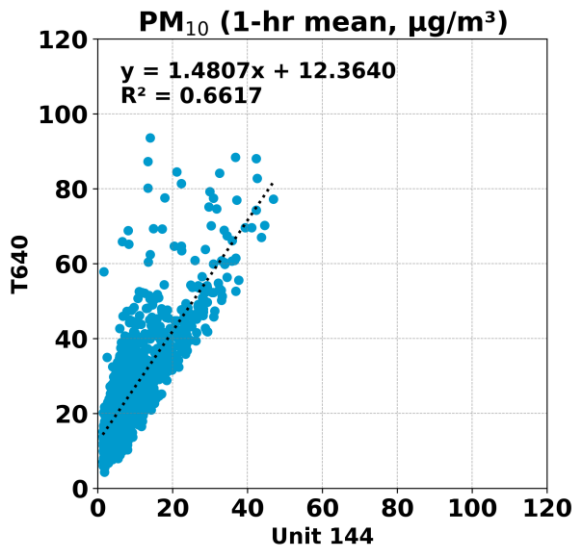


Kunak Air Lite vs T640 (PM_{1.0}; 24-hr mean)

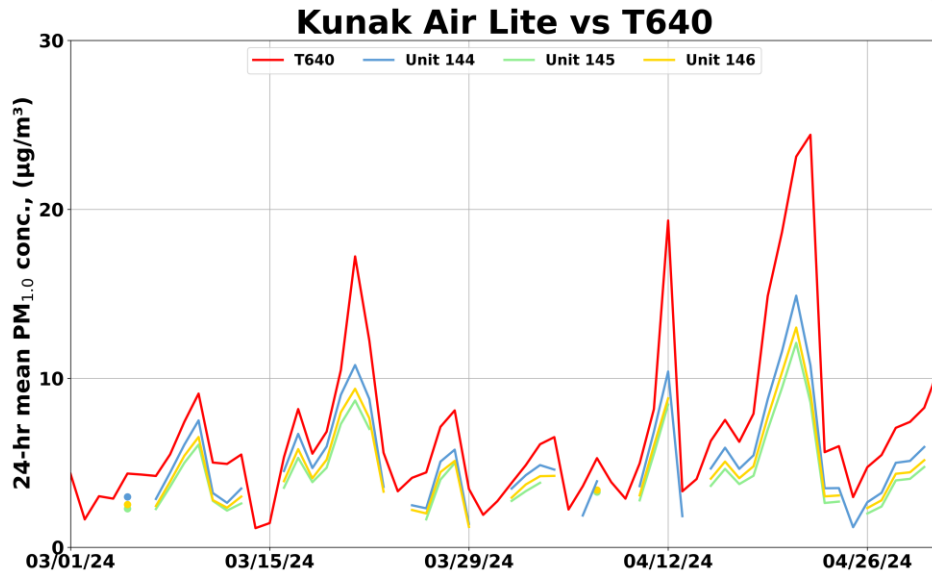




- The Kunak Air Lite sensors showed strong correlations with the corresponding T640 data ($0.87 < R^2 < 0.89$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{1.0} mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM_{1.0} daily variations as recorded by T640

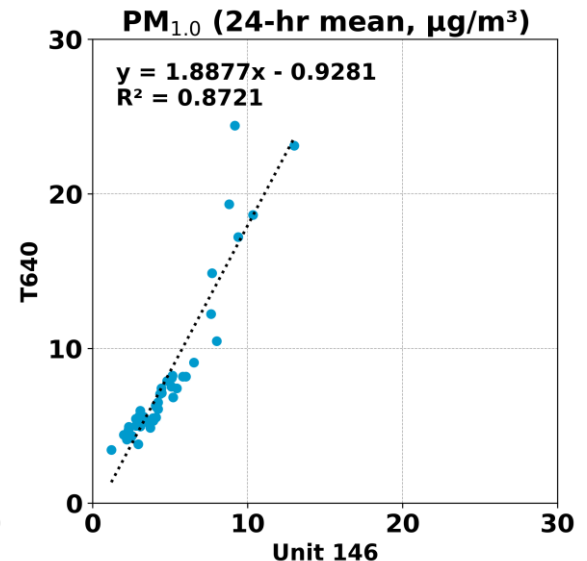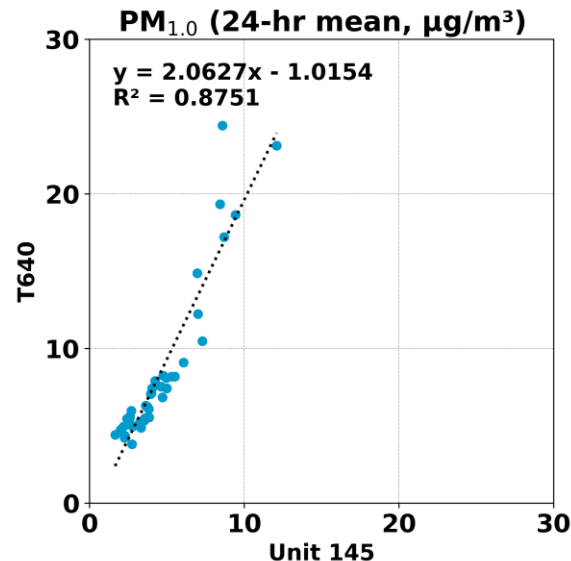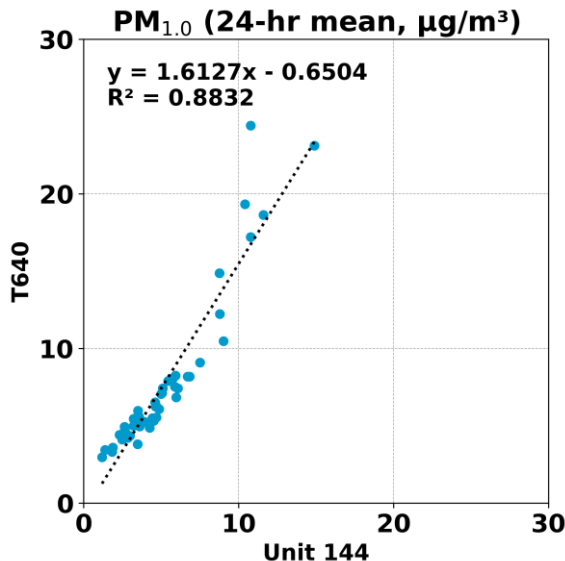


Kunak Air Lite vs FEM T640 (PM_{2.5}; 24-hr mean)

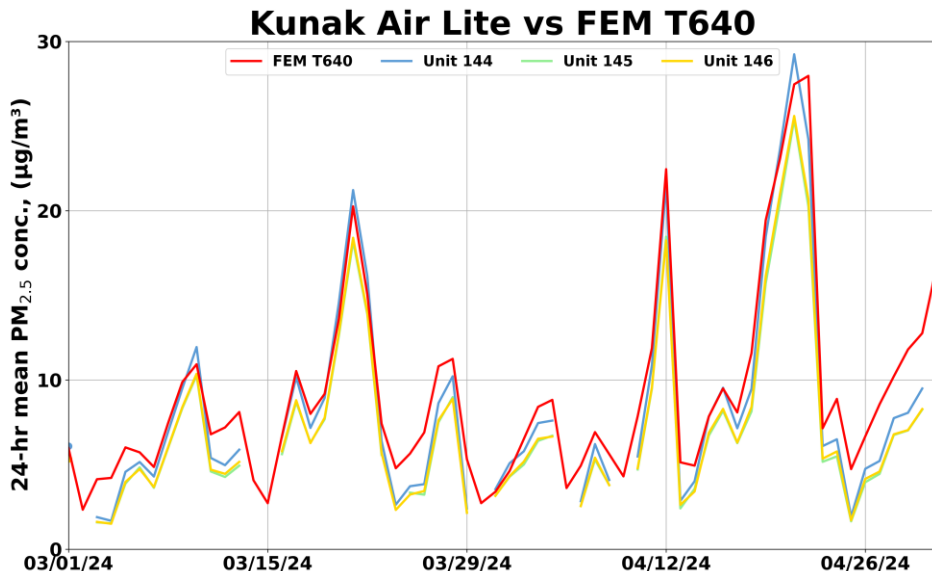




- The Kunak Air Lite sensors showed very strong correlations with the corresponding FEM T640 data ($0.95 < R^2 < 0.96$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{2.5} mass concentrations as measured by FEM T640
- The Kunak Air Lite sensors seemed to track the PM_{2.5} daily variations as recorded by FEM T640

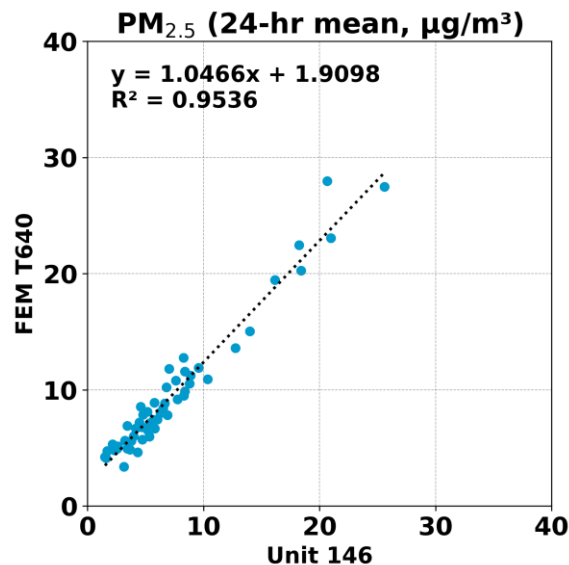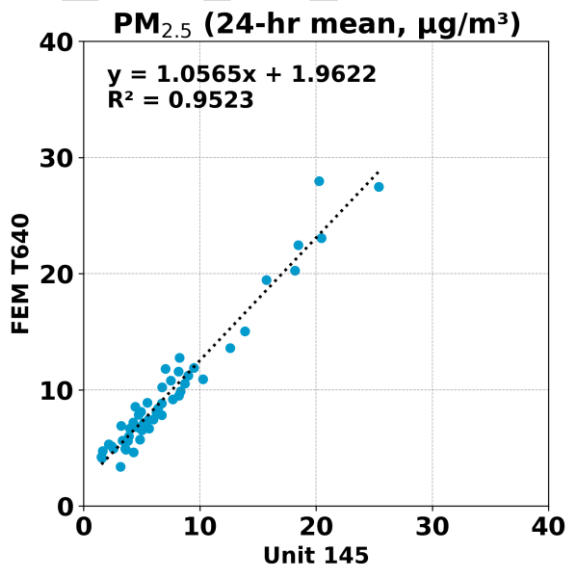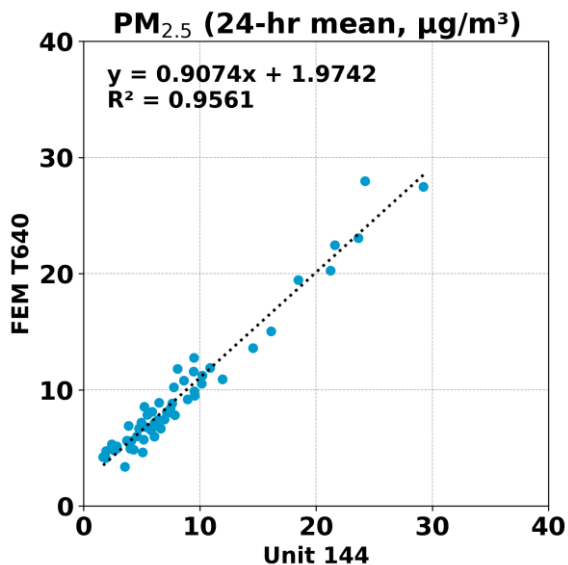


Kunak Air Lite vs T640 (PM₁₀; 24-hr mean)

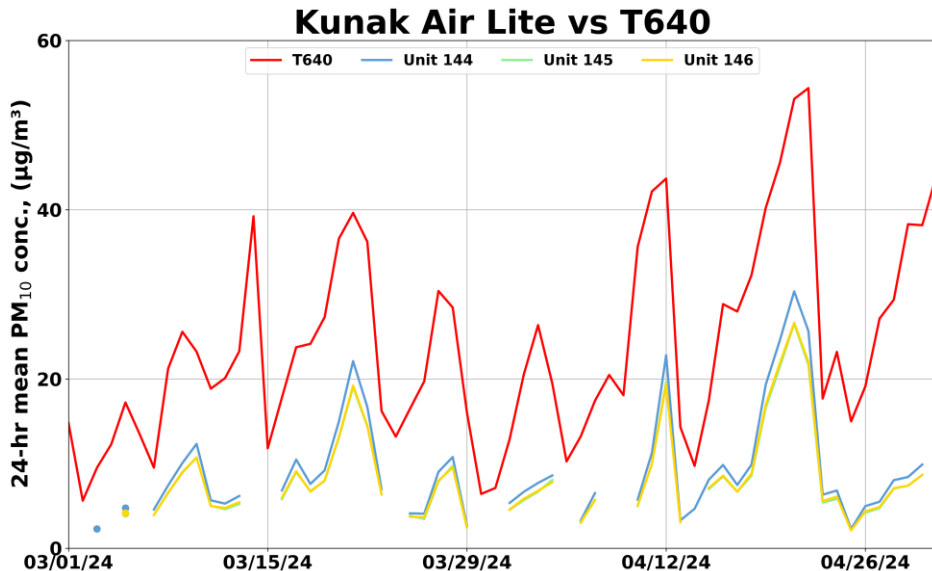




- The Kunak Air Lite sensors showed strong correlations with the corresponding T640 data ($0.72 < R^2 < 0.75$)
- Overall, the Kunak Air Lite sensors underestimated the PM₁₀ mass concentrations as measured by T640
- The Kunak Air Lite sensors seemed to track the PM₁₀ daily variations as recorded by T640

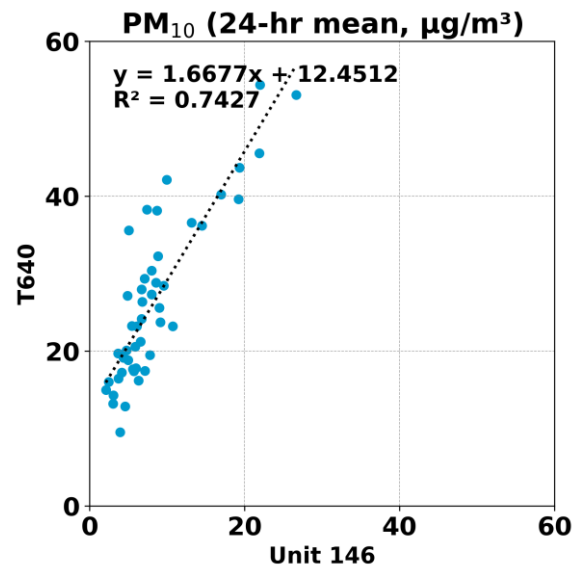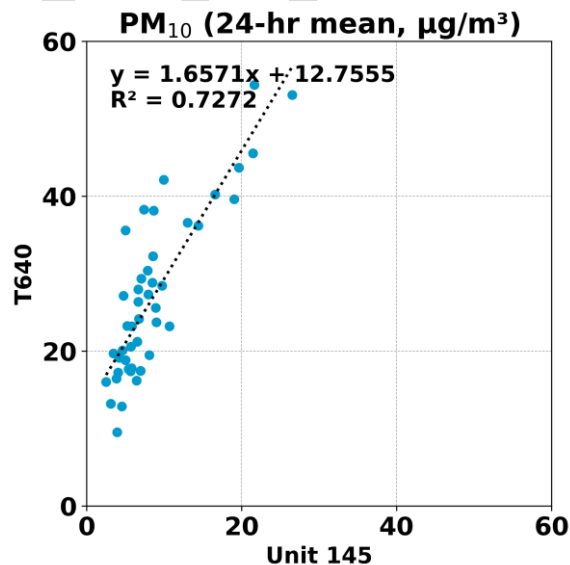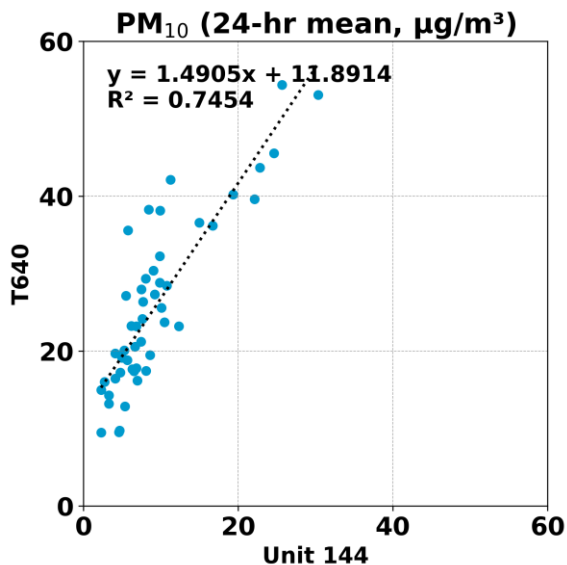


Kunak Air Lite vs FEM BAM (PM_{2.5}; 1-hr mean)

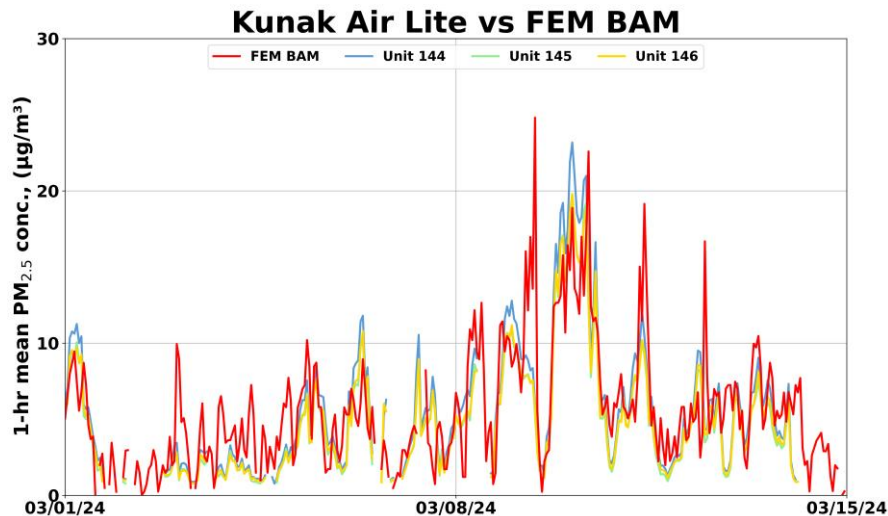




- The Kunak Air Lite sensors showed strong correlations with the corresponding FEM BAM data ($0.70 < R^2 < 0.72$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{2.5} mass concentrations as measured by FEM BAM
- The Kunak Air Lite sensors seemed to track the PM_{2.5} diurnal variations as recorded by FEM BAM

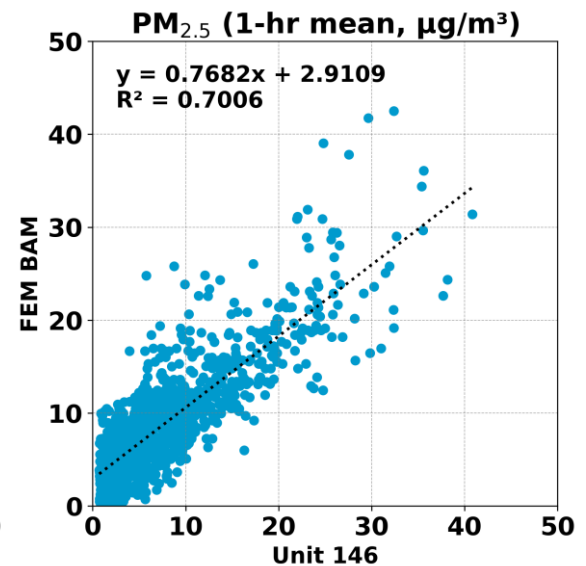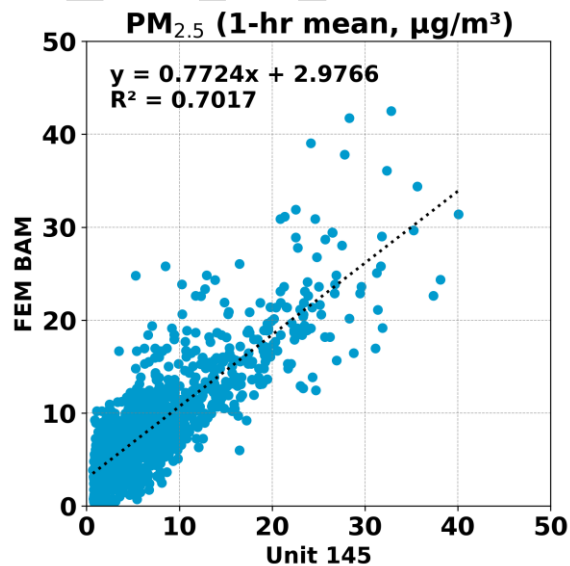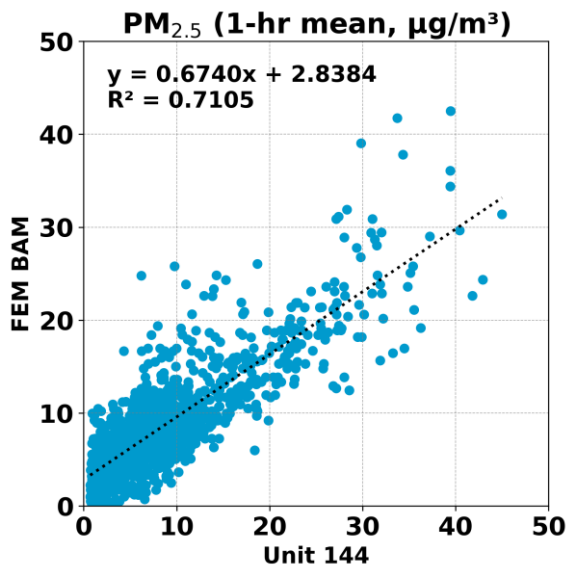


Kunak Air Lite vs FEM BAM (PM₁₀; 1-hr mean)

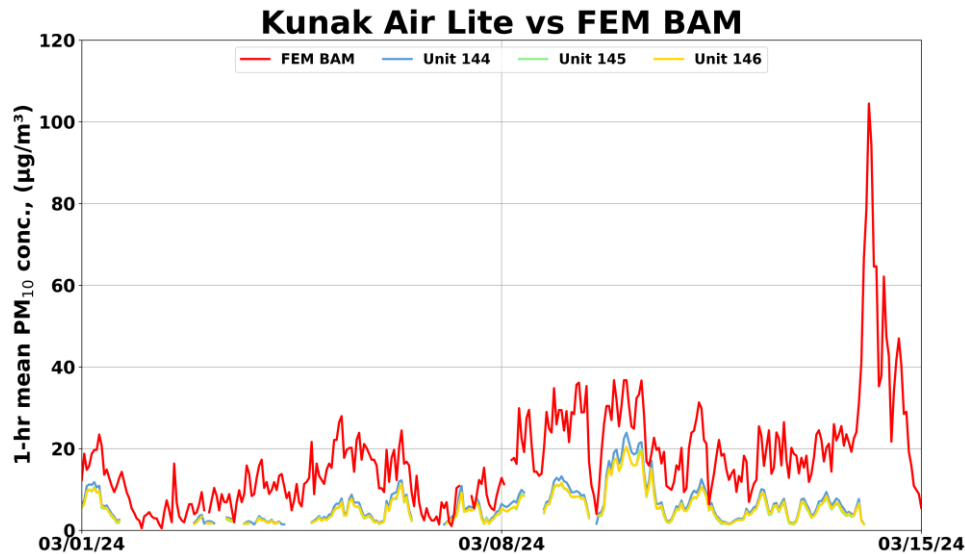




- The Kunak Air Lite sensors showed weak correlations with the corresponding FEM BAM data ($0.40 < R^2 < 0.42$)
- Overall, the Kunak Air Lite sensors underestimated the PM₁₀ mass concentrations as measured by FEM BAM
- The Kunak Air Lite sensors seemed to track the PM₁₀ diurnal variations as recorded by FEM BAM

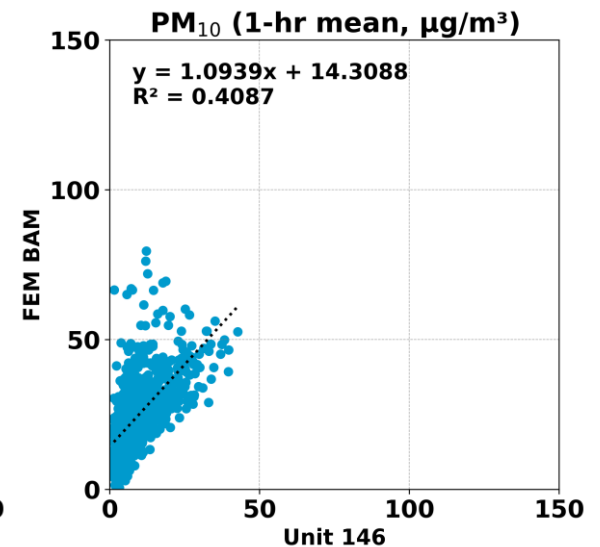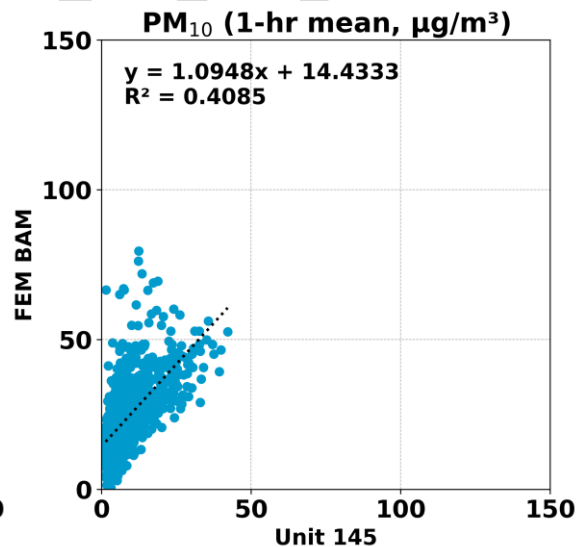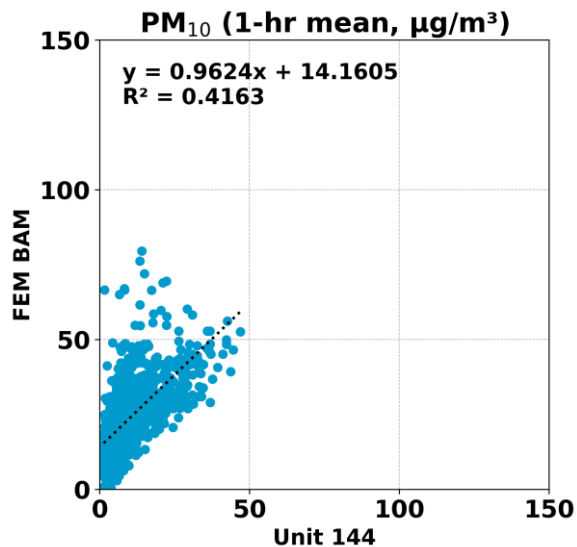


Kunak Air Lite vs FEM BAM (PM_{2.5}; 24-hr mean)

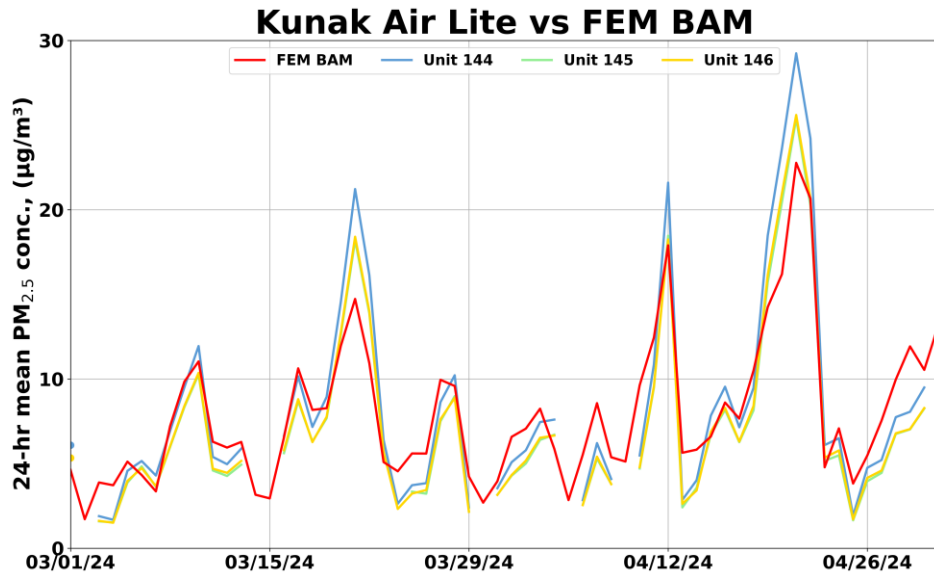




- The Kunak Air Lite sensors showed strong correlations with the corresponding FEM BAM data ($0.89 < R^2 < 0.90$)
- Overall, the Kunak Air Lite sensors underestimated the PM_{2.5} mass concentrations as measured by FEM BAM
- The Kunak Air Lite sensors seemed to track the PM_{2.5} diurnal variations as recorded by FEM BAM

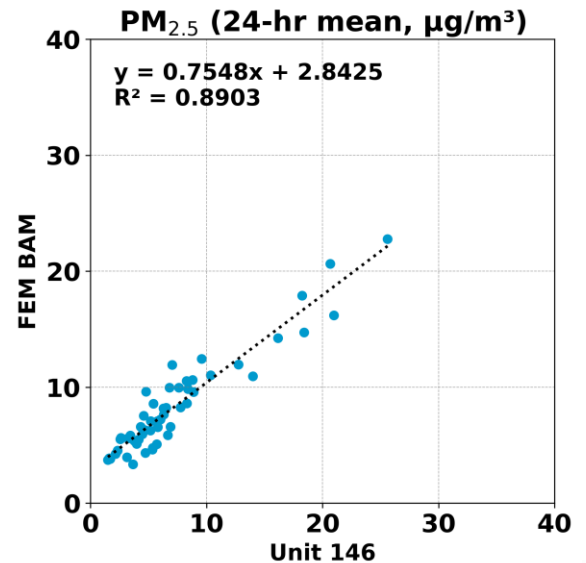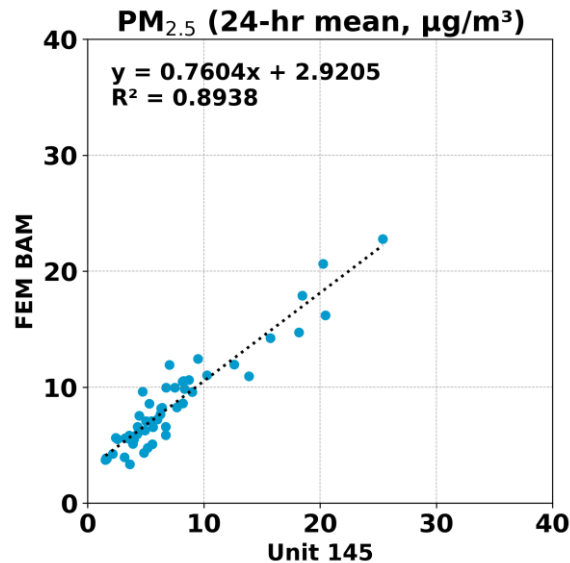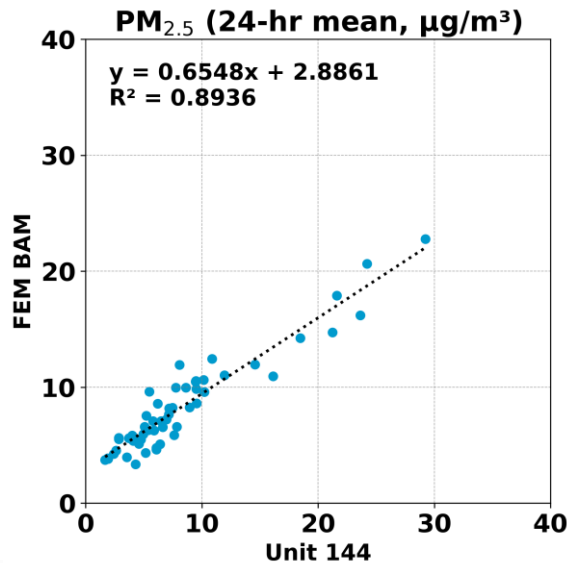

Kunak Air Lite vs FEM BAM (PM₁₀; 24-hr mean)

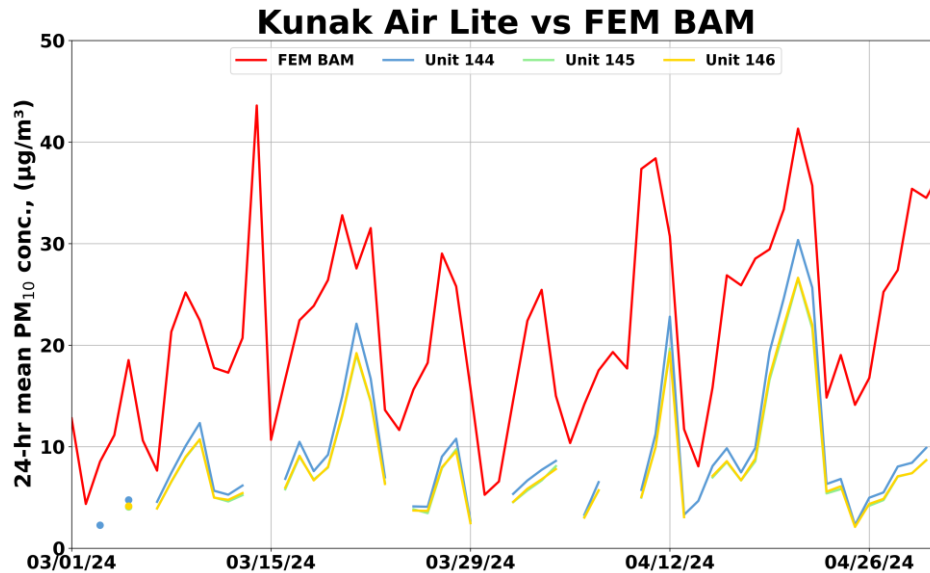

- The Kunak Air Lite sensors showed weak correlations with the corresponding FEM BAM data ($0.45 < R^2 < 0.50$)
- Overall, the Kunak Air Lite sensors underestimated the PM₁₀ mass concentrations as measured by FEM BAM
- The Kunak Air Lite sensors seemed to track the PM₁₀ diurnal variations as recorded by FEM BAM

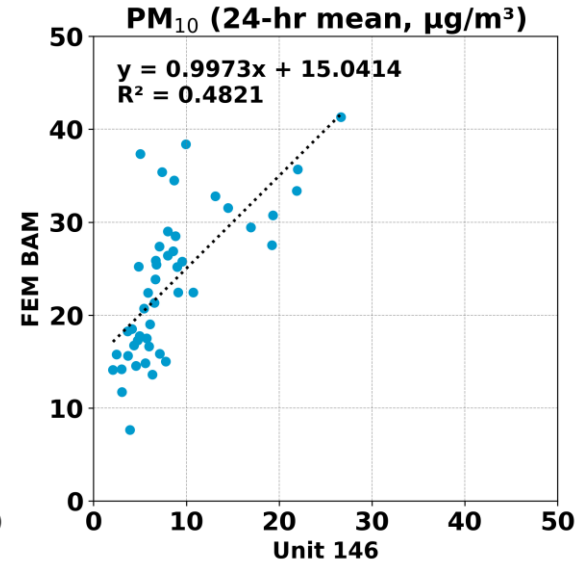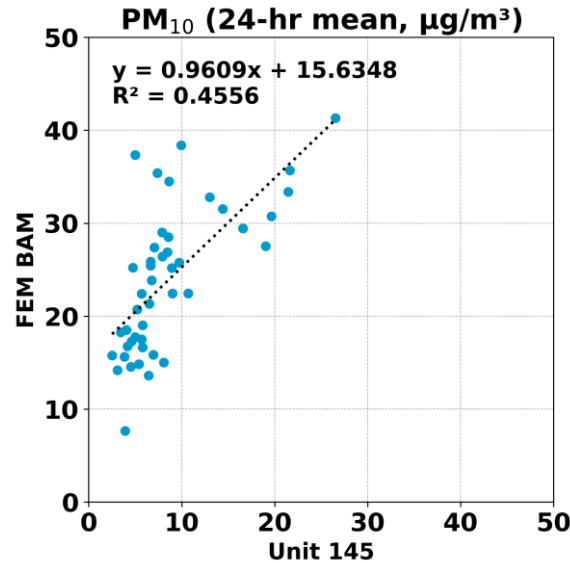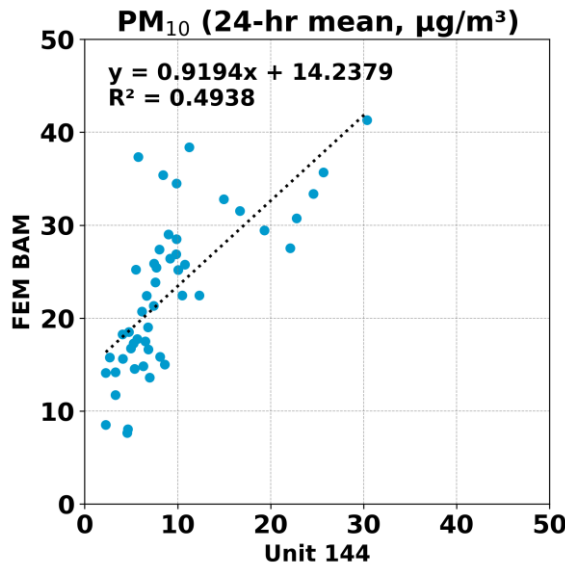

Summary: PM

Average of 3 Sensors, PM _{1.0}		Kunak Air Lite vs T640, PM _{1.0}							T640 (PM _{1.0} , µg/m ³)		
	Average (µg/m ³)	SD (µg/m ³)	R ²	Slope	Intercept	MBE ¹ (µg/m ³)	MAE ² (µg/m ³)	RMSE ³ (µg/m ³)	Ref. Average	Ref. SD	Range during the field evaluation
5-min	4.6	3.3	0.76 to 0.79	1.41 to 1.72	0.5 to 0.8	-3.8 to -2.6	2.6 to 3.8	4.1 to 5.3	6.7	5.9	0.2 to 43.2
1-hr	4.6	3.3	0.77 to 0.80	1.45 to 1.77	0.3 to 0.6	-3.9 to -2.7	2.7 to 3.9	4.1 to 5.3	6.7	5.9	0.3 to 42.0
24-hr	4.9	2.6	0.87 to 0.88	1.61 to 2.06	-1.0 to -0.7	-3.9 to -2.6	2.6 to 3.9	3.6 to 4.9	6.7	4.9	1.1 to 24.4
Average of 3 Sensors, PM _{2.5}		Kunak Air Lite vs FEM BAM & FEM T640, PM _{2.5}							FEM BAM & FEM T640 (PM _{2.5} , µg/m ³)		
	Average (µg/m ³)	SD (µg/m ³)	R ²	Slope	Intercept	MBE ¹ (µg/m ³)	MAE ² (µg/m ³)	RMSE ³ (µg/m ³)	Ref. Average	Ref. SD	Range during the field evaluation
5-min	7.6	6.8	0.88 to 0.90	0.87 to 0.99	2.5 to 2.7	-2.6 to -1.4	2.1 to 2.8	2.7 to 3.5	9.0	6.9	0.1 to 49.5
1-hr	7.7	6.7	0.70 to 0.91	0.67 to 1.01	2.4 to 3.0	-2.6 to -0.1	2.1 to 3.0	2.6 to 4.0	8.0 to 9.0	5.9 to 6.8	0.0 to 47.4
24-hr	7.6	5.5	0.89 to 0.96	0.65 to 1.06	1.9 to 2.9	-2.4 to -0.01	1.5 to 2.4	1.8 to 2.7	7.9 to 9.0	4.3 to 5.7	1.7 to 28.0
Average of 3 Sensors, PM ₁₀		Kunak Air Lite vs FEM BAM & T640, PM ₁₀							FEM BAM & T640 (PM ₁₀ , µg/m ³)		
	Average (µg/m ³)	SD (µg/m ³)	R ²	Slope	Intercept	MBE ¹ (µg/m ³)	MAE ² (µg/m ³)	RMSE ³ (µg/m ³)	Ref. Average	Ref. SD	Range during the field evaluation
5-min	8.4	7.1	0.61 to 0.62	1.47 to 1.67	12.4 to 12.8	-18.2 to -16.7	16.7 to 18.2	19.2 to 20.8	23.9	15.1	0.2 to 138.8
1-hr	8.5	7.0	0.41 to 0.66	0.96 to 1.69	12.4 to 14.4	-18.3 to -13.8	13.9 to 18.3	16.4 to 20.6	21.3 to 23.9	12.6 to 14.7	0.0 to 104.5
24-hr	8.8	5.9	0.46 to 0.75	0.92 to 1.67	11.9 to 15.6	-18.4 to -13.5	13.5 to 18.4	14.7 to 19.6	21.3 to 23.9	9.6 to 11.8	4.4 to 54.4


¹ Mean Bias Error (MBE): the difference between the sensors and the reference instruments. MBE indicates the tendency of the sensors to underestimate (negative MBE values) or overestimate (positive MBE values).

² Mean Absolute Error (MAE): the absolute difference between the sensors and the reference instruments. The larger MAE values, the higher measurement errors as compared to the reference instruments.




³ Root Mean Square Error (RMSE): another metric to calculate measurement errors.

Kunak Air Lite vs South Coast AQMD Met Station (Temp; 5-min mean)

Kunak Air Lite vs. South Coast AQMD Met Station

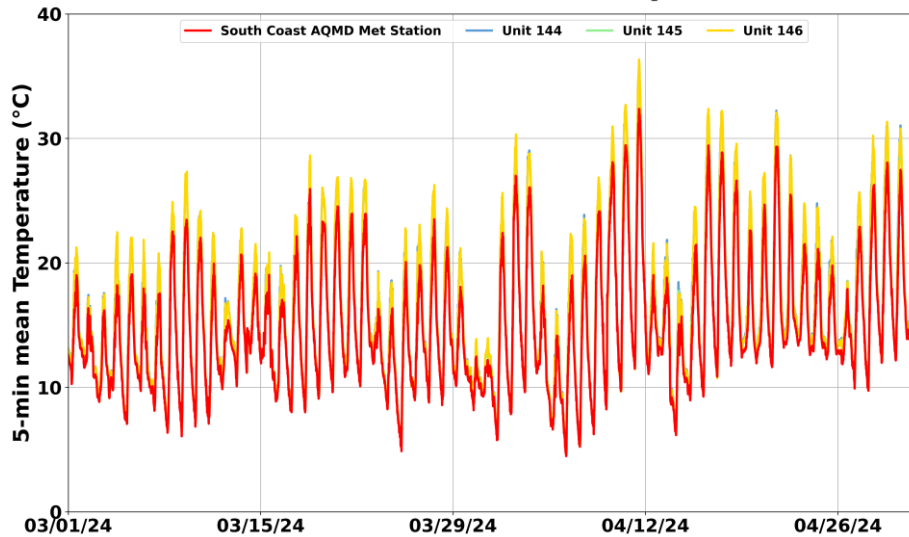


- The Kunak Air Lite sensors showed very strong correlations with the corresponding South Coast AQMD Met Station data ($0.97 < R^2 < 0.99$)
- Overall, the Kunak Air Lite sensors overestimated the temperature measurement as recorded by South Coast AQMD Met Station
- The Kunak Air Lite sensors seemed to track the diurnal temperature variations as recorded by South Coast AQMD Met Station

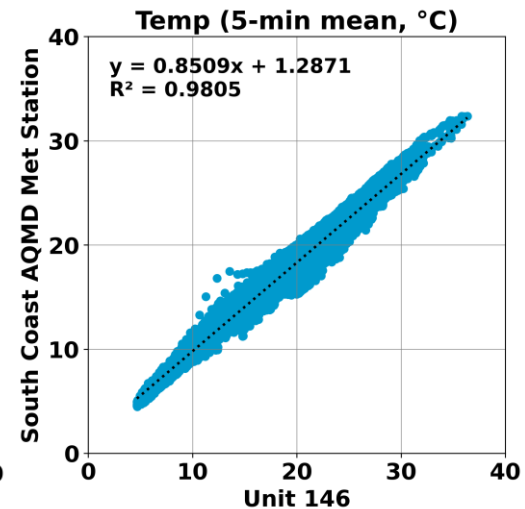
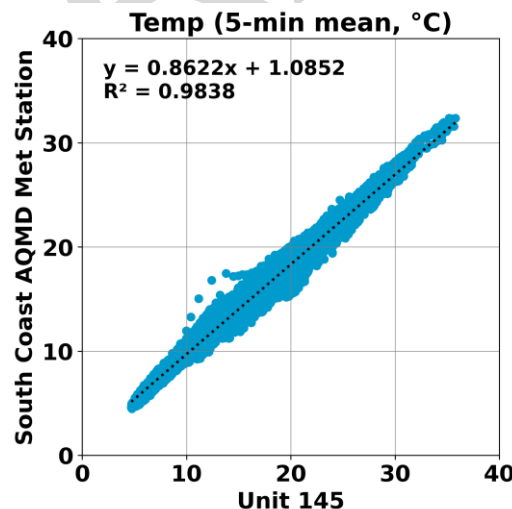
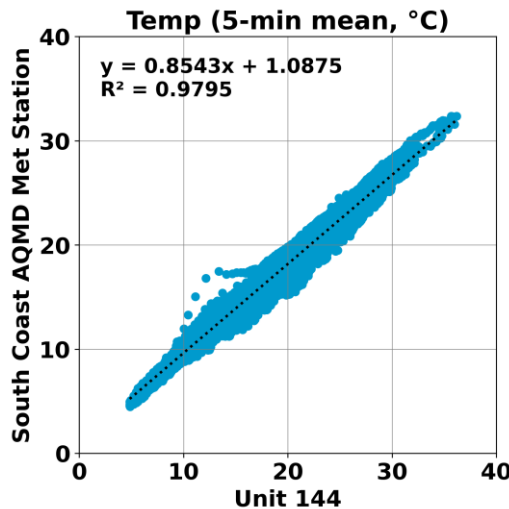


Kunak Air Lite vs South Coast AQMD Met Station (RH; 5-min mean)

Kunak Air Lite vs. South Coast AQMD Met Station

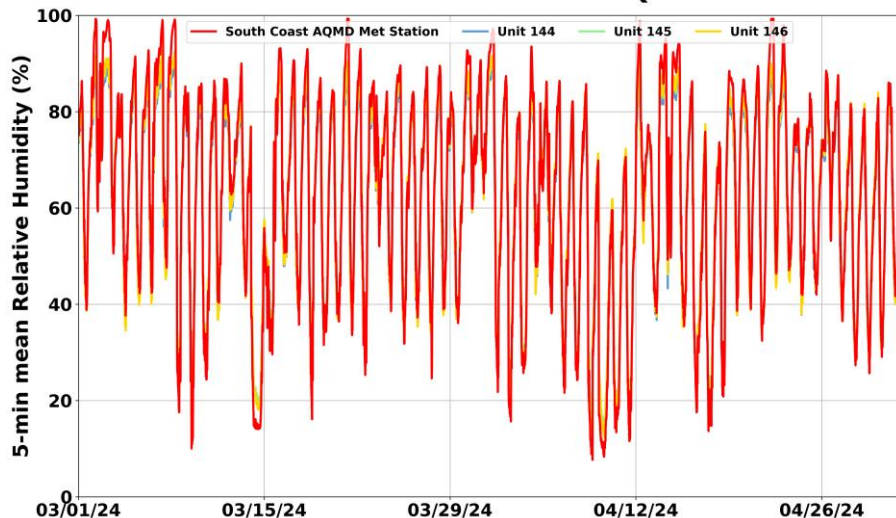

- Kunak Air Lite sensors showed very strong correlations with the corresponding South Coast AQMD Met Station data ($0.98 < R^2 < 0.99$)
- Overall, the Kunak Air Lite sensors underestimated the RH measurement as recorded by South Coast AQMD Met Station
- The Kunak Air Lite sensors seemed to track the diurnal RH variations as recorded by South Coast AQMD Met Station

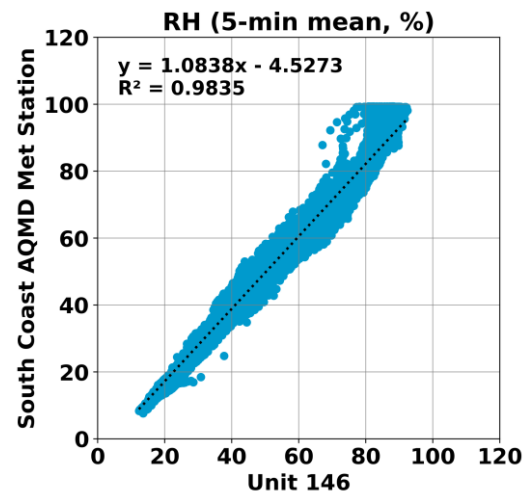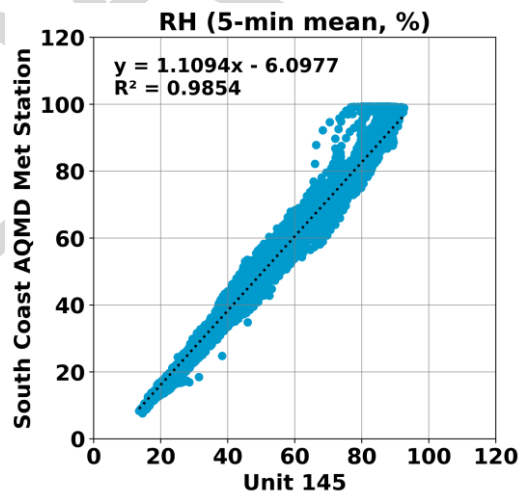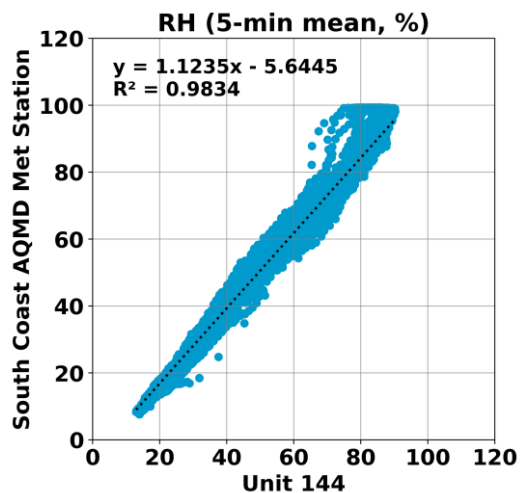

Discussion

- The three **Kunak Air Lite** sensors' data recovery for O₃, NO₂ and all PM fractions was ~99.0%, 99.1% and 99.7%, respectively.
- The absolute intra-model variability for O₃ and NO₂ was ~1.09 ppb and ~0.41 ppb, respectively. Absolute intra-model variability was ~ 0.57, ~0.68 and ~0.72 µg/m³ for PM_{1.0}, PM_{2.5} and PM₁₀, respectively
- Reference instruments: strong correlations between FEM BAM and FEM T640 for PM_{2.5} (R² ~ 0.77, 1-hr mean) and strong correlations between FEM BAM and T640 for PM₁₀ (R² ~ 0.83, 1-hr mean) mass concentration measurements
- During the entire field deployment testing period:
 - Ozone sensors showed strong correlation with the FEM T400 instrument (0.84 < R² < 0.89, 5-min mean) and generally underestimated the corresponding FEM T400 data
 - NO₂ sensors showed moderate correlations with the FRM T200 instrument (0.66 < R² < 0.70, 5-min mean) and overestimated the corresponding FRM T200 data
 - The Kunak Air Lite sensors showed strong correlations with the corresponding reference PM_{1.0} data (0.77 < R² < 0.80, 1-hr mean), strong to very strong correlations with the corresponding reference PM_{2.5} data (0.70 < R² < 0.92, 1-hr mean) and weak to moderate correlations with the corresponding reference PM₁₀ data (0.4 < R² < 0.67; 1-hr mean). The sensors underestimated PM_{1.0}, PM_{2.5} and PM₁₀ mass concentrations as measured by the reference instruments
 - Temperature and relative humidity sensors showed very strong correlations with the South Coast AQMD Met Station T and RH data, respectively (R² ~ 0.98 for T and R² ~ 0.98 for RH) and overestimated the T and underestimated the RH data as recorded by the South Coast AQMD Met Station
- No sensor calibration was performed by South Coast AQMD staff for this evaluation.
- Laboratory chamber testing is necessary to fully evaluate the performance of these sensors under controlled T and RH conditions, and known target and interferent pollutants concentrations.
- These results are still preliminary